
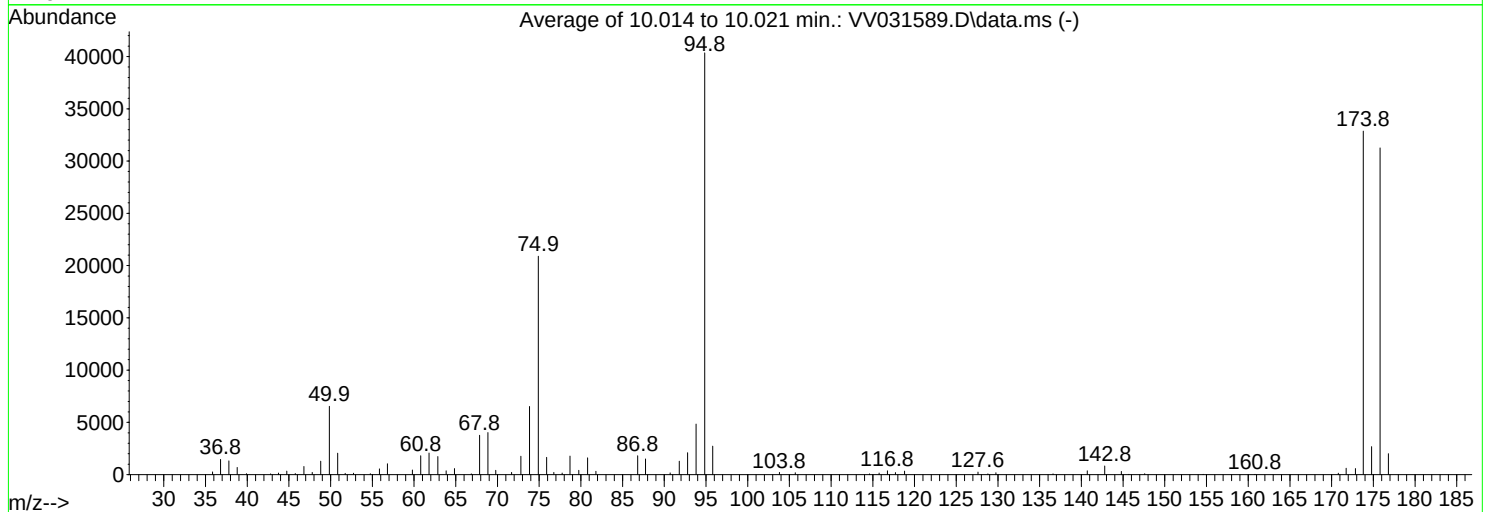


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031589.D
Acq On : 19 Jun 2023 08:55
Operator : SY/MD
Sample : BFB390
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB390

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Thu Jun 22 02:14:12 2023

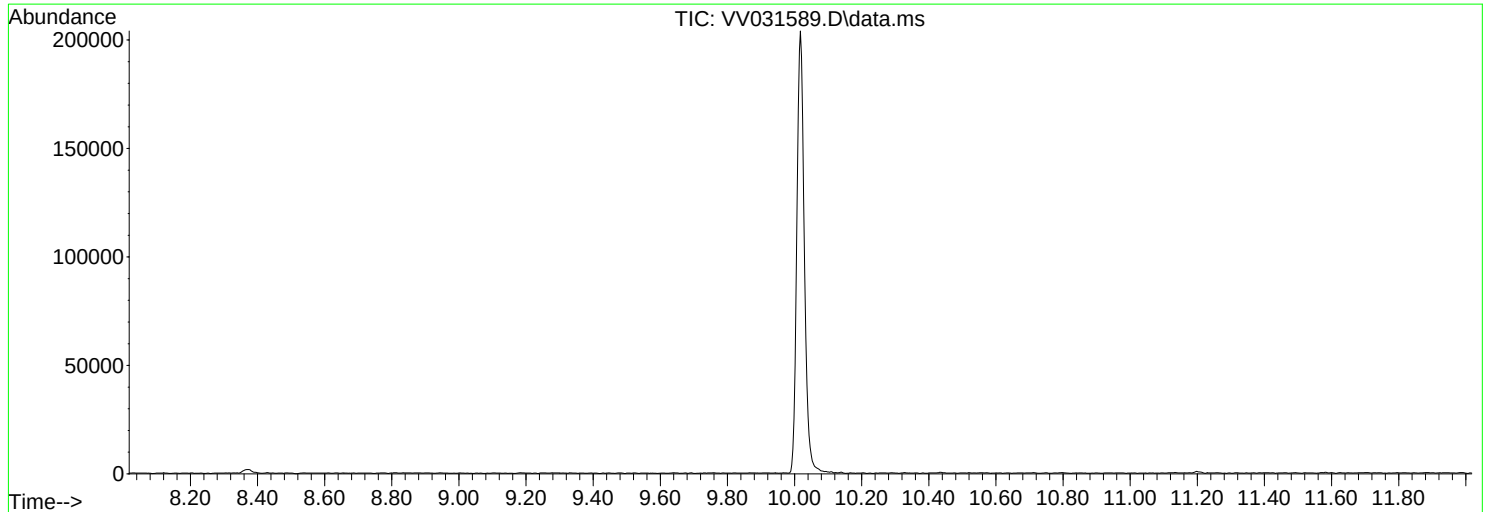

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	6545	PASS
75	95	30	80	51.8	20896	PASS
95	95	100	100	100.0	40352	PASS
96	95	5	9	6.8	2728	PASS
173	174	0.00	2	1.8	579	PASS
174	95	50	120	81.4	32864	PASS
175	174	5	9	8.1	2676	PASS
176	174	95	105	95.1	31253	PASS
177	176	5	10	6.4	2007	PASS

m/z	Abundance
39.70	153.0
43.80	248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
35.80	225.0
36.80	1394.0
37.80	1329.0
38.80	671.0
39.70	120.0
43.70	380.0
44.70	294.0
46.80	799.0
47.80	220.0
48.80	1353.0
49.80	6540.0
50.80	2011.0
51.70	107.0
52.70	128.0
55.90	545.0
56.80	1130.0
59.80	412.0
60.80	1866.0
61.80	2096.0
62.90	1782.0
63.90	375.0
64.90	551.0
66.90	120.0
67.90	3818.0
68.90	4017.0
69.80	423.0
71.70	216.0
72.80	1804.0
73.80	6309.0
74.90	21120.0
75.90	1764.0
76.80	208.0
77.80	148.0
78.70	1774.0
79.70	372.0
80.80	1503.0
81.80	344.0
86.80	1837.0
87.70	1595.0
90.70	171.0
91.80	1435.0
92.80	2075.0
93.80	4709.0
94.80	40072.0
95.80	2688.0
103.80	202.0
105.70	182.0
114.60	131.0
115.70	191.0
116.70	350.0
117.70	202.0
118.80	317.0
127.60	246.0
129.80	199.0
140.70	378.0
142.80	831.0
144.80	286.0
145.70	118.0
147.60	146.0
170.80	140.0
171.80	537.0
172.80	562.0
173.80	31944.0
174.80	2562.0
175.80	30680.0
176.80	2014.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
35.90	256.0
36.80	1501.0
37.80	1354.0
38.80	731.0
39.90	117.0
42.80	126.0
43.70	403.0
44.80	343.0
45.80	144.0
46.80	839.0
47.80	223.0
48.80	1323.0
49.90	6779.0
50.90	2115.0
51.70	118.0
52.80	140.0
54.70	130.0
55.90	563.0
56.80	1090.0
59.80	478.0
60.80	1875.0
61.80	2156.0
62.80	1760.0
63.70	369.0
64.80	613.0
66.80	116.0
67.80	3890.0
68.80	4134.0
69.80	427.0
71.70	227.0
72.80	1801.0
73.90	6731.0
74.90	21608.0
75.90	1683.0
76.70	217.0
77.80	157.0
78.70	1829.0
79.80	415.0
80.80	1635.0
81.80	342.0
86.80	1848.0
87.70	1567.0
90.70	174.0
91.80	1333.0
92.80	2201.0
93.80	4987.0
94.80	41640.0
95.80	2780.0
103.80	218.0
105.70	203.0
114.60	115.0
115.70	156.0
116.70	385.0
117.70	207.0
118.80	366.0
127.60	240.0
128.80	117.0
129.80	182.0
136.60	118.0
140.70	379.0
142.80	848.0
144.80	303.0
147.60	132.0
154.60	108.0
160.80	115.0
170.80	148.0
171.80	631.0
172.90	623.0
173.80	34112.0
174.80	2810.0
175.80	32280.0
176.80	2059.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
35.80	289.0
36.80	1475.0
37.80	1248.0
38.80	664.0
39.90	143.0
42.80	109.0
43.80	427.0
44.80	359.0
45.70	192.0
46.80	709.0
47.80	218.0
48.80	1187.0
49.90	6317.0
50.90	2020.0
51.80	129.0
52.80	133.0
54.80	137.0
55.80	523.0
56.80	908.0
59.80	456.0
60.80	1686.0
61.80	1940.0
62.80	1632.0
63.90	346.0
64.80	577.0
67.80	3601.0
68.80	3911.0
69.80	390.0
71.70	210.0
72.80	1657.0
73.90	6527.0
74.90	19960.0
75.90	1525.0
76.70	224.0
77.70	172.0
78.70	1720.0
79.80	455.0
80.80	1668.0
81.80	278.0
86.80	1715.0
87.80	1356.0
90.70	161.0
91.80	1106.0
92.80	2027.0
93.80	4799.0
94.90	39344.0
95.80	2717.0
103.80	212.0
105.70	187.0
115.80	120.0
116.80	366.0
117.70	190.0
118.80	350.0
127.60	227.0
128.80	126.0
129.70	174.0
136.60	112.0
140.70	343.0
142.80	796.0
144.80	326.0
170.80	137.0
171.70	650.0
172.90	553.0
173.80	32536.0
174.80	2657.0
175.80	30800.0
176.80	1948.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390