

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062019\
 Data File : VV011619.D
 Acq On : 19 Jun 2019 14:34
 Operator : SY/MD
 Sample : K3415-18
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GALQ3

Quant Time: Jun 20 03:14:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 20 02:04:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	168026	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	155948	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	63847	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	64924	5.12	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.40%
7) Chloroethane-d5	1.55	69	44171	5.49	ug/L	-0.03
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.80%
11) 1,1-Dichloroethene-d2	2.12	63	92918	3.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.00%
20) 2-Butanone-d5	3.94	46	158309	44.35	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.70%
24) Chloroform-d	4.40	84	112736	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.08	65	65630	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	5.09	84	236414	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.12	67	71819	4.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.20%
41) Toluene-d8	7.36	98	206966	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
43) trans-1,3-Dichloropropene-	7.66	79	21488	4.37	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.40%
46) 2-Hexanone-d5	8.13	63	113415	39.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.98%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	46850	4.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	68063	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	24013	9.982 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062019\
Data File : VV011619.D
Acq On : 19 Jun 2019 14:34
Operator : SY/MD
Sample : K3415-18
Misc : 25ML/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GALQ3

Quant Time: Jun 20 03:14:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 20 02:04:09 2019
Response via : Initial Calibration

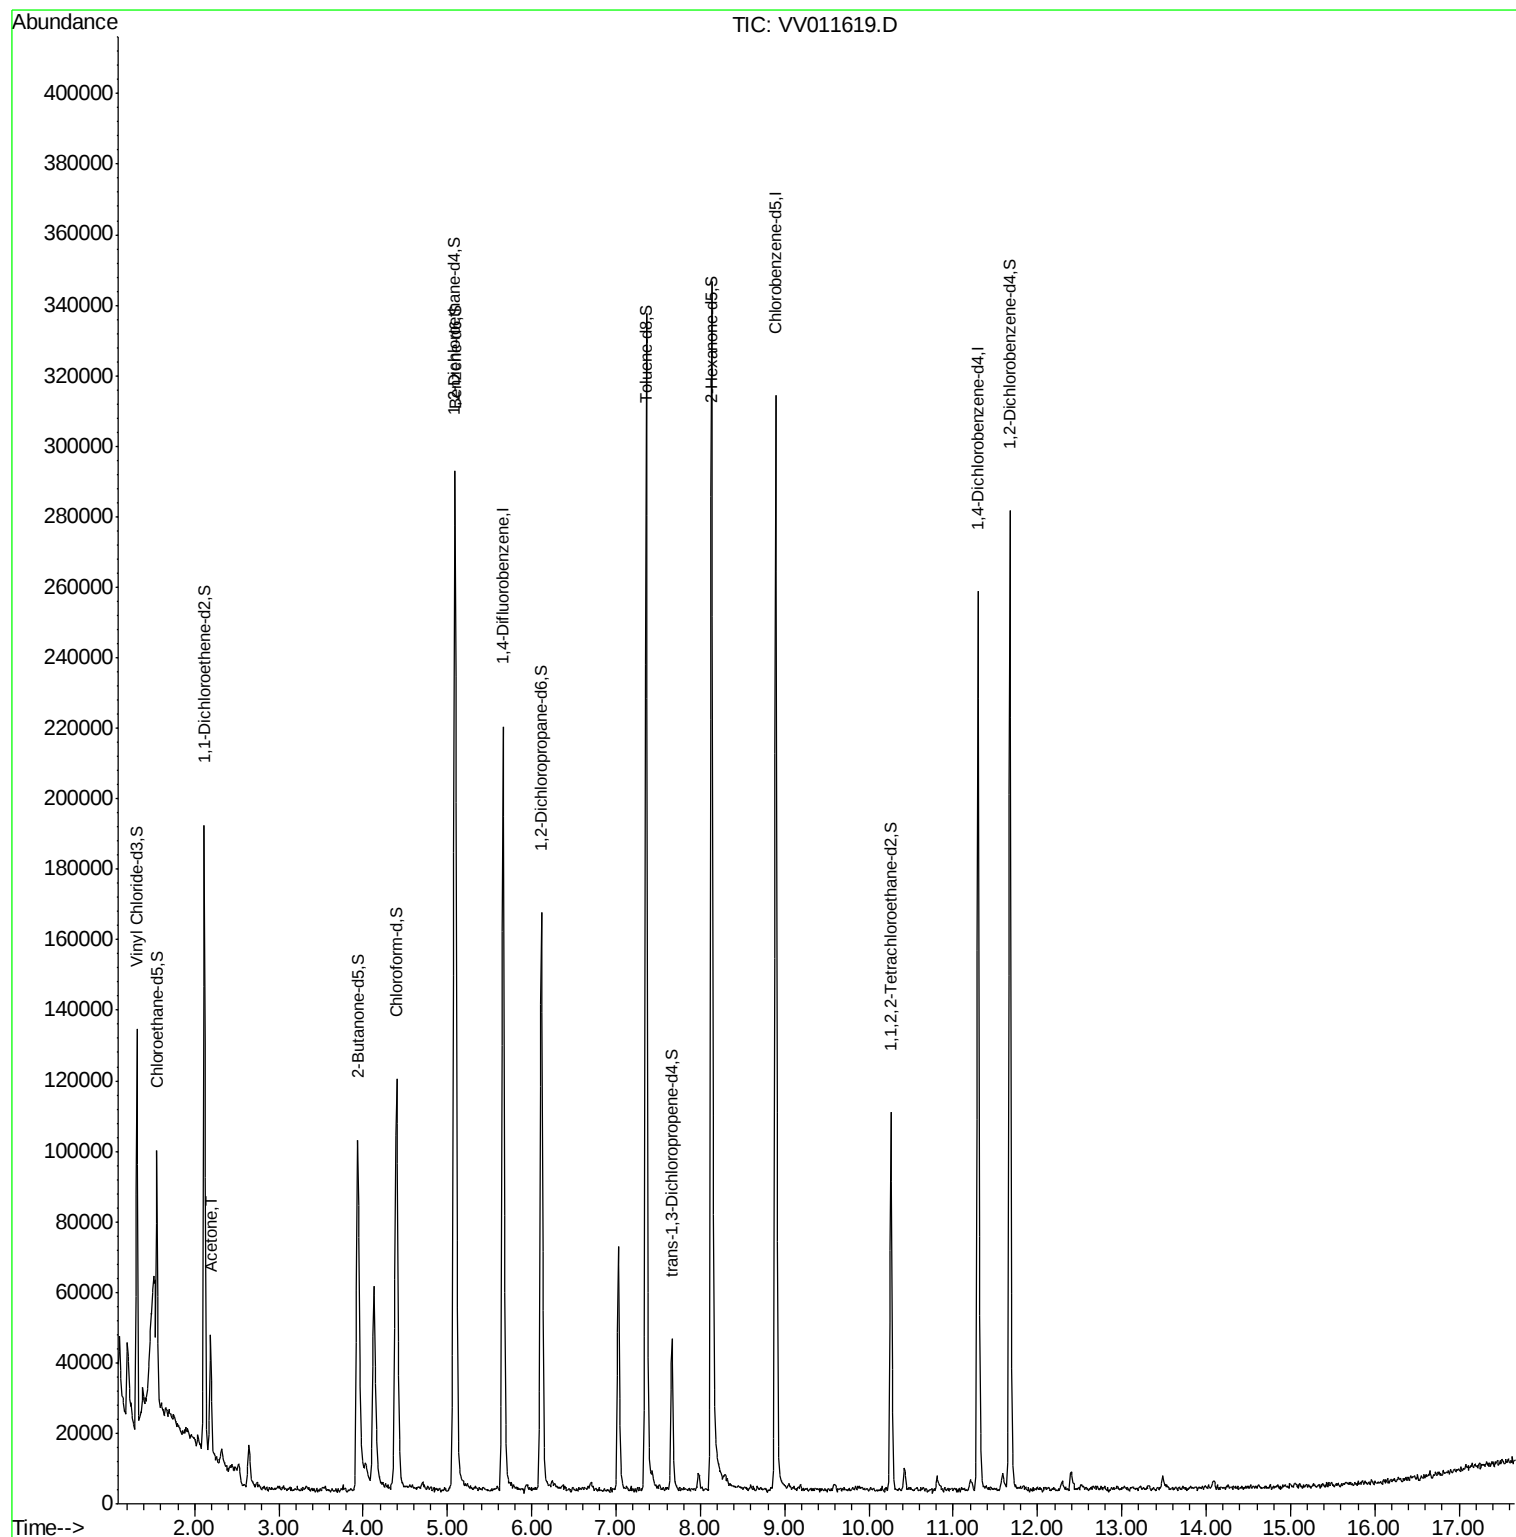

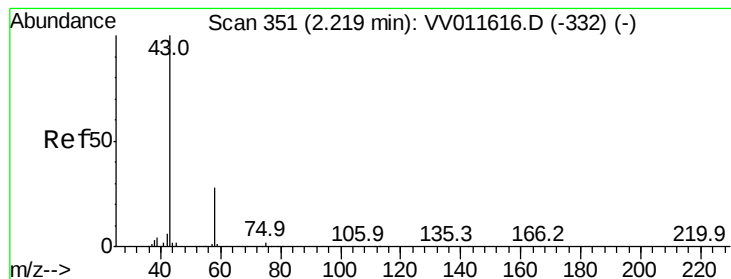

#13

Acetone

Concen: 9.982 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.03 min

Lab File: VV011619.D

Acq: 19 Jun 2019 14:34

Instrument :
MSVOA_V
ClientSampleId :
GALQ3

Tot Ion: 43 Resp: 24013

Ion Ratio Lower Upper

43 100

58 28.8 0.0 57.8

