

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062019\
 Data File : VV011620.D
 Acq On : 19 Jun 2019 15:00
 Operator : SY/MD
 Sample : K3415-19
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GALQ4

Quant Time: Jun 20 03:16:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 20 02:04:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	156838	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	148368	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	61407	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65045	5.50	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.00%
7) Chloroethane-d5	1.55	69	43921	5.85	ug/L	-0.03
Spiked Amount	5.000	Range	65 - 130	Recovery	=	117.00%
11) 1,1-Dichloroethene-d2	2.12	63	91829	4.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.40%
20) 2-Butanone-d5	3.94	46	158609	47.60	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.20%
24) Chloroform-d	4.39	84	108116	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.08	65	62979	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
32) Benzene-d6	5.09	84	234395	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.80%
36) 1,2-Dichloropropane-d6	6.11	67	70792	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.36	98	205270	5.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.00%
43) trans-1,3-Dichloropropene-	7.66	79	21297	4.55	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.00%
46) 2-Hexanone-d5	8.13	63	119592	44.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.64%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	46782	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	67692	5.52	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	24965	11.118 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062019\
Data File : VV011620.D
Acq On : 19 Jun 2019 15:00
Operator : SY/MD
Sample : K3415-19
Misc : 25ML/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GALQ4

Quant Time: Jun 20 03:16:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 20 02:04:09 2019
Response via : Initial Calibration

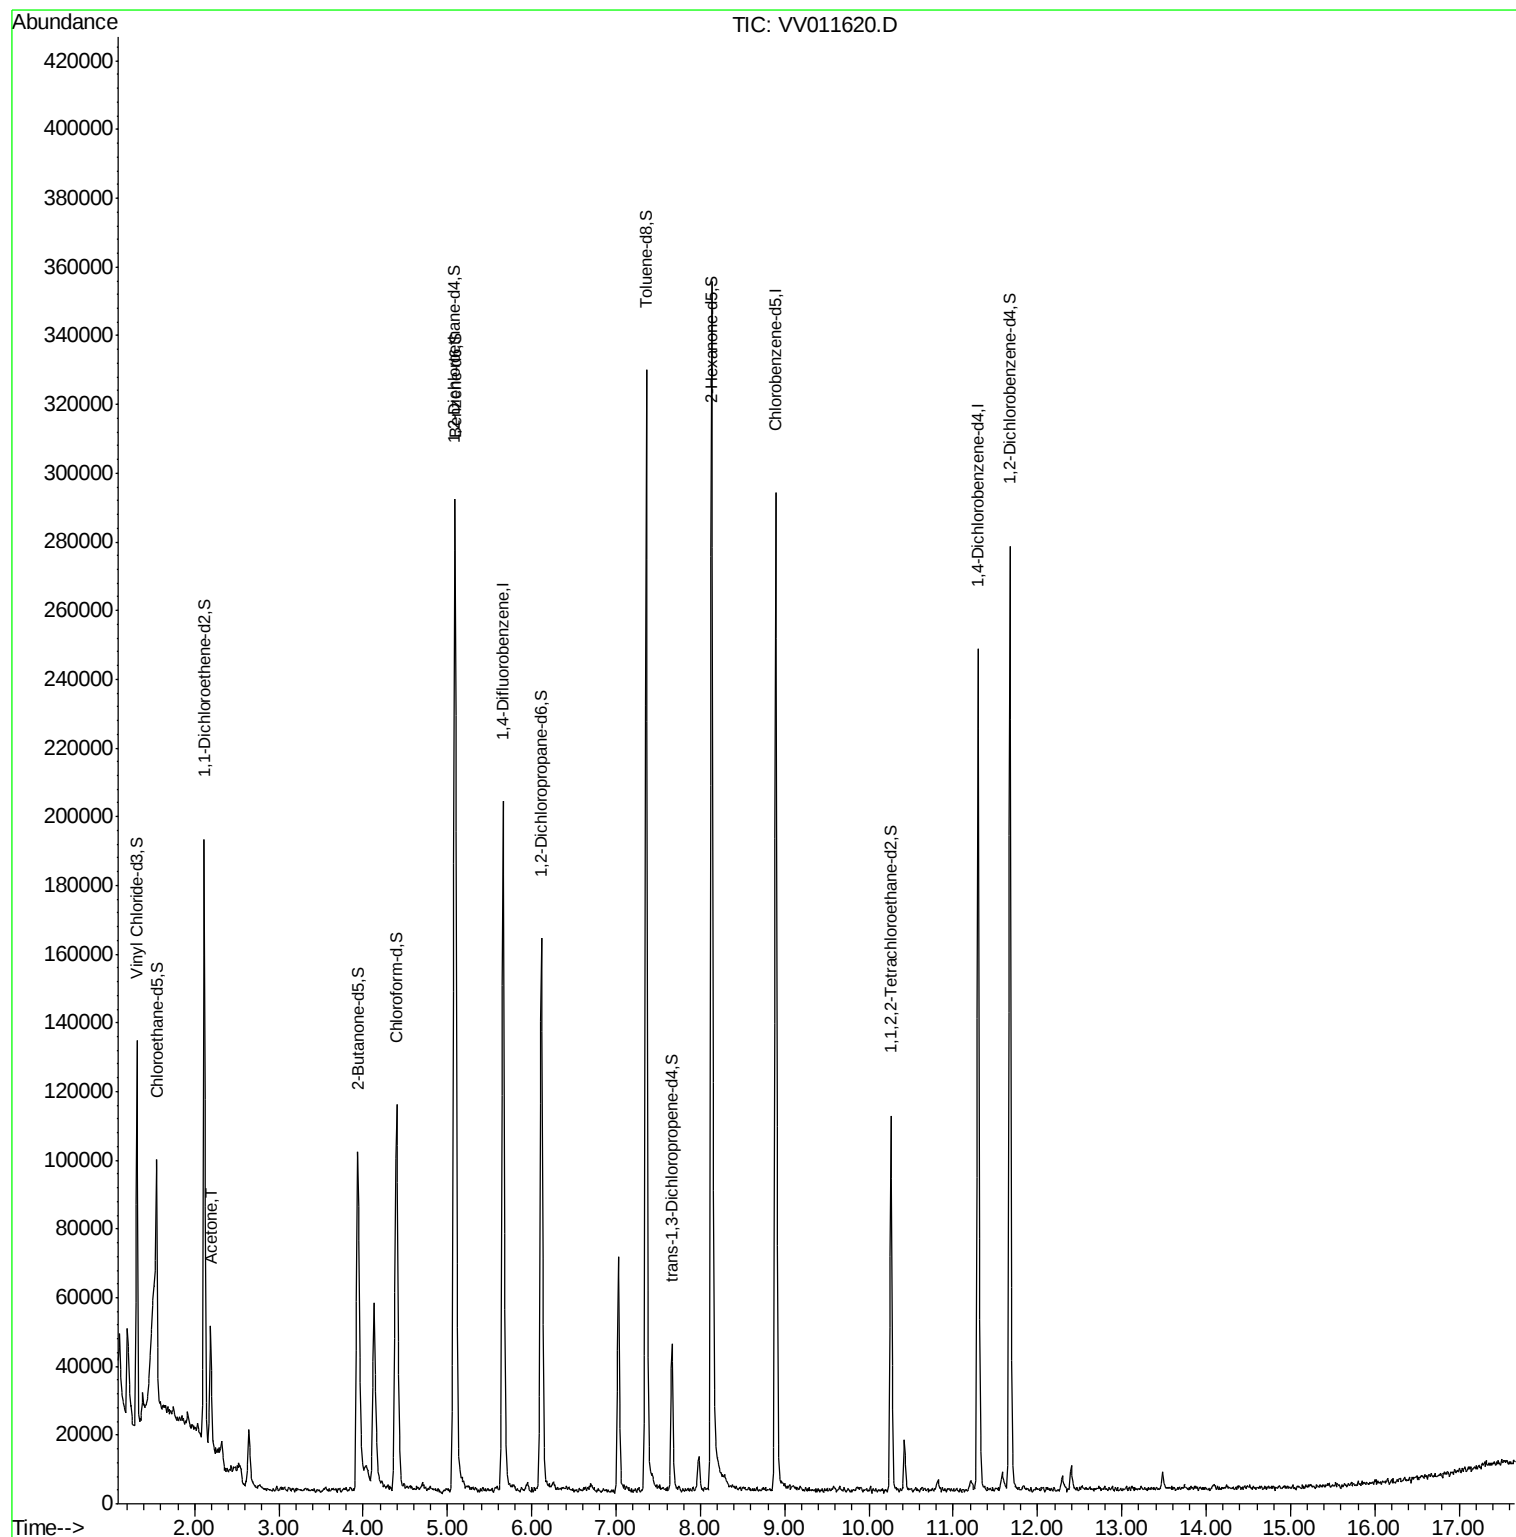

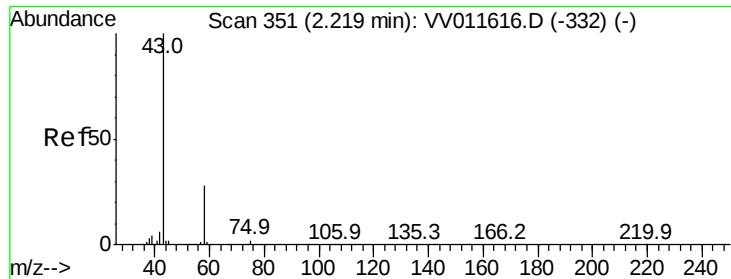

#13
Acetone
Concen: 11.118 ug/L
RT: 2.19 min Scan# 342
Delta R.T. -0.03 min
Lab File: VV011620.D
Acq: 19 Jun 2019 15:00

Instrument :
MSVOA_V
ClientSampleId :
GALQ4

Tot Ion: 43 Resp: 24965
Ion Ratio Lower Upper
43 100
58 29.2 0.0 57.8

