


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062019\
 Data File : VV011615.D
 Acq On : 19 Jun 2019 11:38
 Operator : SY/MD
 Sample : BFB52
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB52

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jun 20 02:04:09 2019

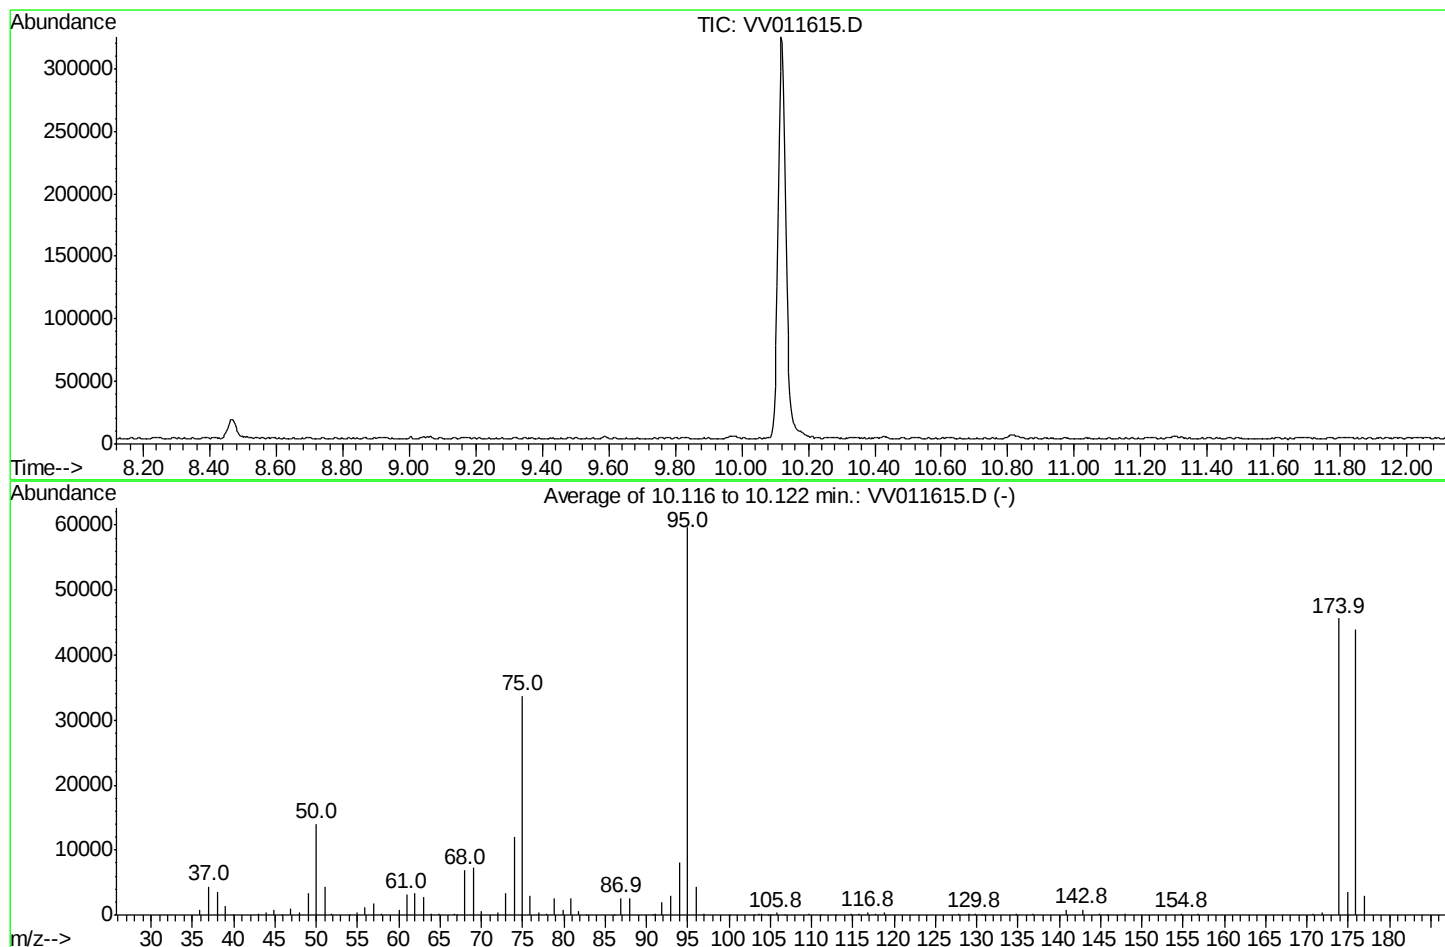

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	14068	PASS
75	95	30	80	56.5	33701	PASS
95	95	100	100	100.0	59669	PASS
96	95	5	9	7.3	4373	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.5	45658	PASS
175	174	5	9	7.6	3483	PASS
176	174	95	101	96.4	43997	PASS
177	176	5	9	6.8	2971	PASS

Scan 2795 (10.077 min): VV011615.D
BFB52

m/z	Abundance
35.70	134.0
37.50	107.0
38.00	111.0
38.90	109.0
39.90	2329.0
41.10	124.0
42.80	106.0
43.90	1236.0
45.80	122.0
47.30	103.0
47.90	141.0
60.80	109.0
64.00	116.0
79.10	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
35.80	818.0
37.00	4126.0
38.00	3563.0
39.00	1595.0
39.90	2447.0
43.00	140.0
44.00	1594.0
44.90	805.0
45.90	233.0
46.90	1027.0
48.00	444.0
49.00	3206.0
50.00	13331.0
51.00	4158.0
51.90	211.0
54.90	308.0
55.90	1170.0
57.00	1794.0
57.90	145.0
60.00	873.0
61.00	3168.0
62.00	3189.0
63.00	2660.0
63.90	398.0
64.90	262.0
66.80	267.0
68.00	6585.0
69.00	7152.0
70.00	647.0
71.90	478.0
73.00	3210.0
74.00	11357.0
75.00	32144.0
75.90	2979.0
76.90	480.0
77.90	240.0
78.90	2518.0
79.90	766.0
80.90	2254.0
81.80	567.0
86.90	2583.0
87.90	2376.0
90.80	316.0
91.90	1887.0
93.00	2830.0
94.00	7613.0
95.00	56632.0
96.00	4166.0
97.10	180.0
103.00	119.0
103.70	385.0
105.00	112.0
105.80	338.0
106.70	128.0
109.70	123.0
112.90	125.0
114.90	136.0
115.80	256.0
116.90	434.0
117.80	296.0
118.80	385.0
127.80	176.0
129.00	137.0
129.80	268.0
130.90	101.0
134.80	197.0
136.70	239.0
140.90	783.0
142.90	813.0
144.80	151.0
145.80	130.0
148.00	174.0
154.90	194.0
156.80	108.0
170.80	172.0
171.80	430.0
173.90	42760.0
174.90	3470.0
175.90	40424.0
176.90	2706.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
35.90	863.0
37.00	4544.0
38.00	3858.0
39.00	1534.0
39.90	2397.0
40.90	109.0
42.70	129.0
43.10	142.0
44.00	1611.0
44.90	792.0
45.90	218.0
46.90	1117.0
47.90	485.0
49.00	3528.0
50.00	14551.0
51.00	4486.0
51.90	240.0
54.90	312.0
55.90	1263.0
57.00	1886.0
57.80	160.0
60.00	850.0
61.00	3495.0
62.00	3473.0
63.00	2817.0
63.90	423.0
64.90	300.0
66.80	228.0
68.00	7178.0
69.00	7579.0
70.00	665.0
72.00	489.0
73.00	3441.0
74.00	12390.0
75.00	34880.0
75.90	3187.0
76.90	479.0
77.80	273.0
78.80	2578.0
79.90	853.0
80.90	2529.0
81.80	629.0
82.70	123.0
86.10	124.0
86.90	2718.0
87.90	2599.0
91.00	299.0
91.90	2008.0
93.00	3036.0
94.00	8460.0
95.00	61544.0
96.00	4504.0
96.90	212.0
100.10	110.0
103.00	102.0
103.90	377.0
105.80	342.0
106.70	109.0
109.70	133.0
111.10	129.0
114.80	149.0
115.70	290.0
116.80	489.0
117.70	308.0
118.90	467.0
127.80	220.0
129.10	195.0
129.80	302.0
130.60	107.0
130.90	105.0
134.80	160.0
136.70	197.0
140.90	812.0
142.80	858.0
144.80	170.0
145.80	105.0
148.00	178.0
154.90	215.0
156.70	142.0
170.80	137.0
171.80	472.0
173.90	47152.0
174.90	3580.0
175.90	45560.0
176.90	3057.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
35.90	859.0
37.00	4354.0
38.00	3681.0
39.00	1371.0
39.90	2438.0
40.90	126.0
42.80	141.0
43.10	151.0
44.00	1621.0
44.90	747.0
45.80	182.0
46.90	964.0
47.90	506.0
49.00	3392.0
50.00	14322.0
51.00	4313.0
51.90	277.0
54.00	100.0
54.90	315.0
55.90	1233.0
57.00	1794.0
57.80	165.0
60.00	737.0
61.00	3421.0
62.00	3531.0
63.00	2791.0
63.90	429.0
64.90	287.0
67.00	229.0
68.00	7123.0
69.00	7375.0
70.00	616.0
72.00	442.0
73.00	3311.0
74.00	12115.0
75.00	34080.0
76.00	2947.0
76.90	435.0
77.80	314.0
78.80	2387.0
79.90	879.0
80.90	2667.0
81.80	578.0
82.70	127.0
86.10	170.0
86.90	2667.0
87.90	2627.0
91.00	325.0
91.90	1957.0
93.00	2909.0
94.00	8253.0
95.00	60832.0
96.00	4451.0
96.80	237.0
100.10	101.0
104.00	378.0
104.70	103.0
105.80	364.0
109.80	117.0
111.00	161.0
114.80	145.0
115.70	298.0
116.80	475.0
117.70	297.0
118.90	449.0
127.70	242.0
129.00	190.0
129.80	304.0
130.70	152.0
134.80	123.0
136.80	152.0
140.90	783.0
142.80	838.0
144.90	167.0
148.00	168.0
154.80	219.0
156.80	145.0
170.80	111.0
171.80	438.0
173.90	47064.0
174.90	3400.0
175.90	46008.0
176.90	3151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52