
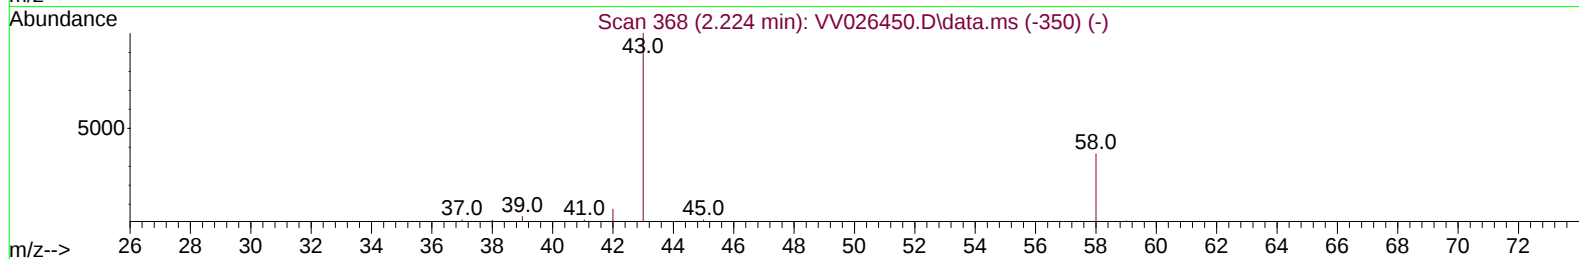
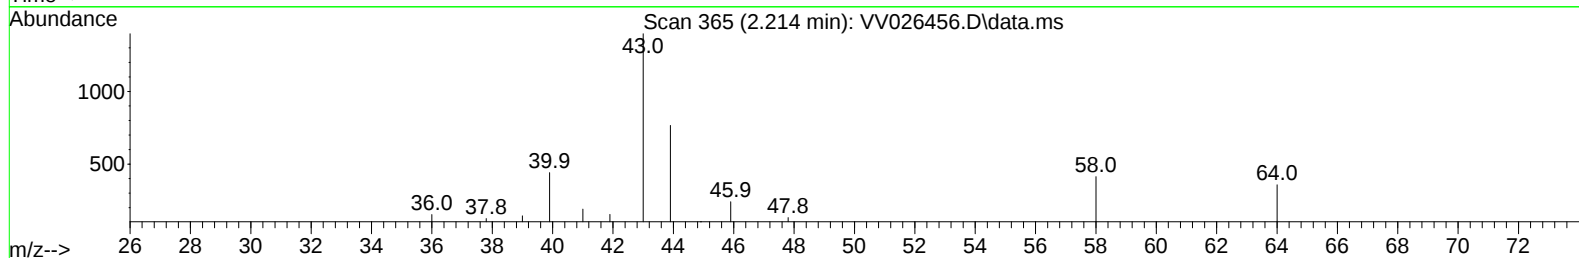


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026456.D
 Acq On : 20 Jun 2022 19:25
 Operator : SY/MD
 Sample : N3385-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: Jun 21 05:39:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

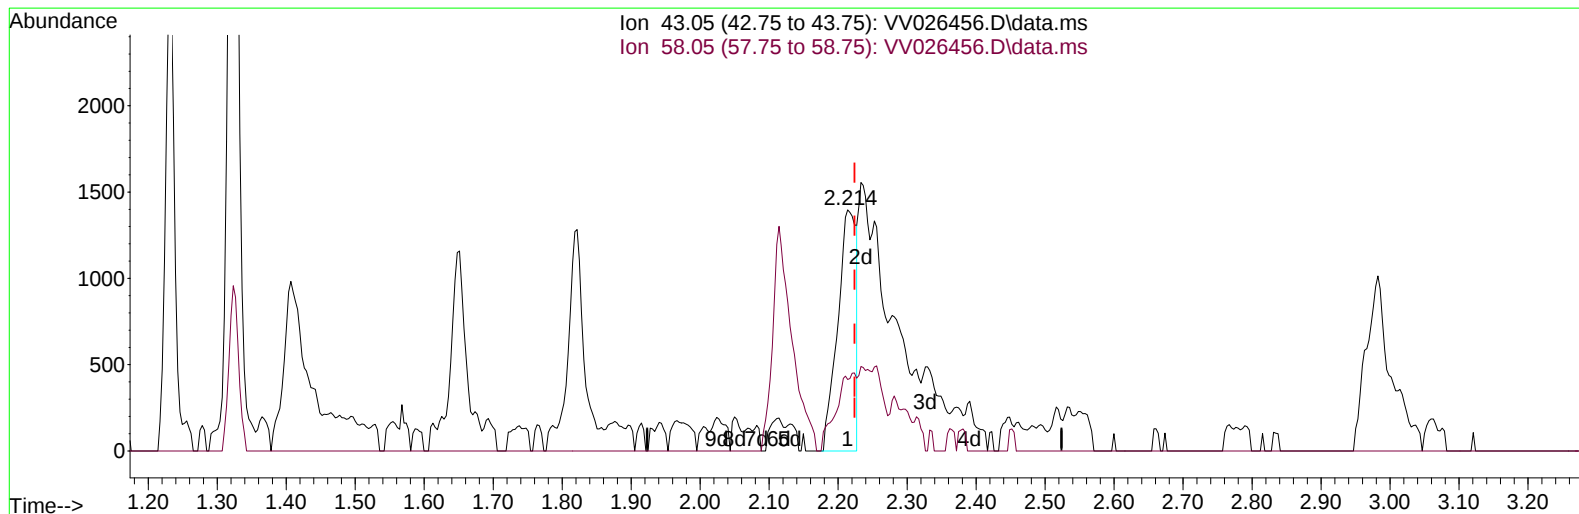

TIC: VV026456.D\data.ms

(13) Acetone (T)

2.214min (-0.010) 2.88 ug/L

response 2590

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	22.78
0.00	0.00	0.00
0.00	0.00	0.00