




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026441.D
 Acq On : 20 Jun 2022 13:18
 Operator : SY/MD
 Sample : N3358-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/21/2022

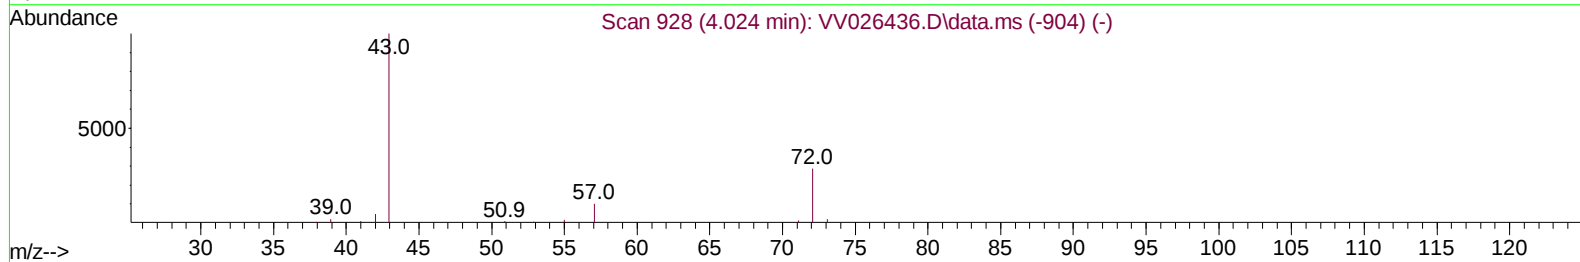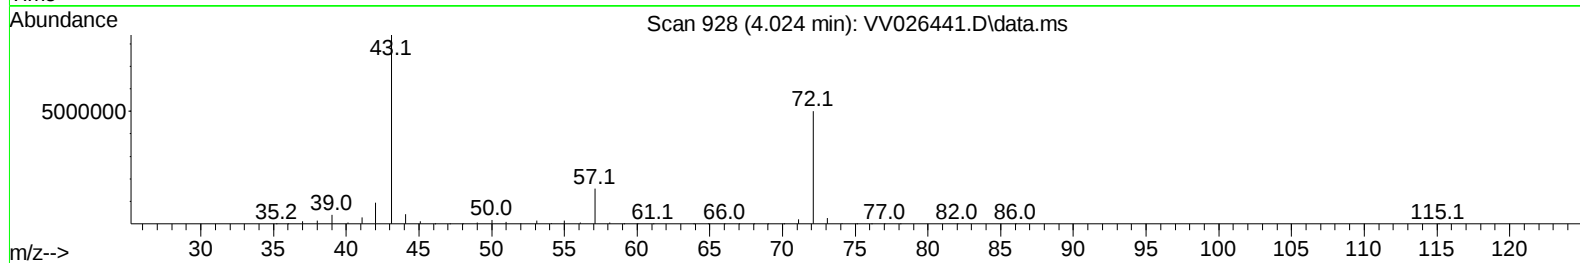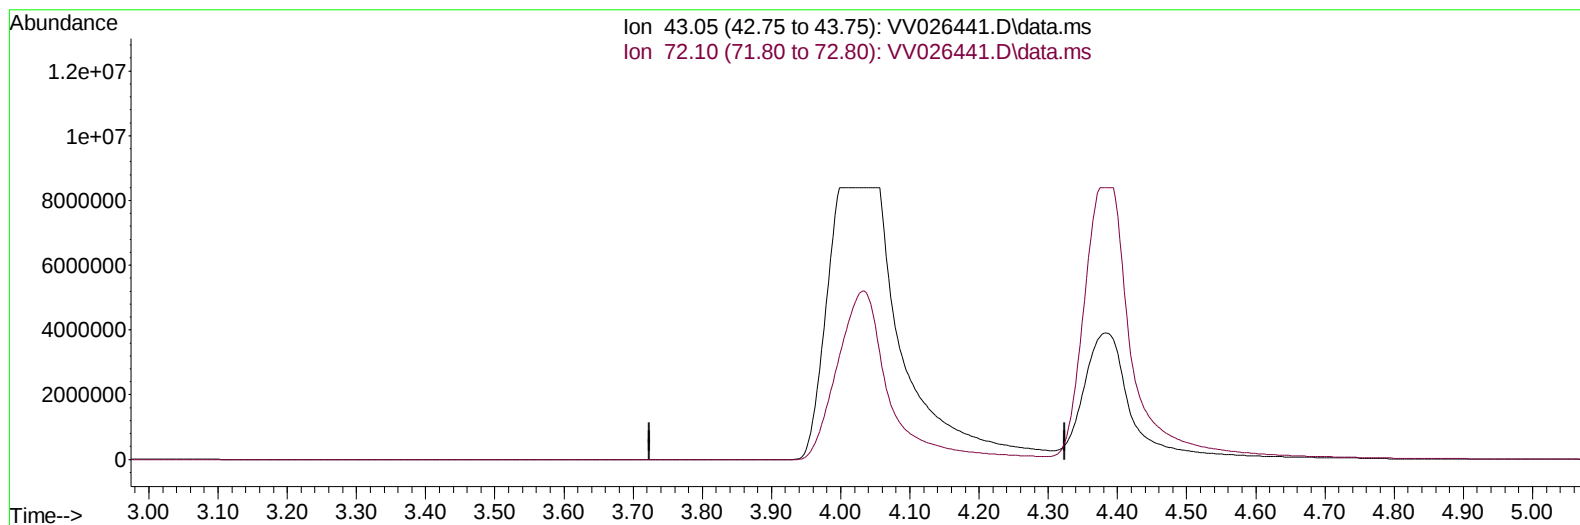

TIC: VV026441.D\data.ms

(21) 2-Butanone (T)

4.024min (-4.024) 0.00 ug/L

response 0

Ion	Exp%	Act%
43.05	100.00	0.00
72.10	25.30	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026441.D
 Acq On : 20 Jun 2022 13:18
 Operator : SY/MD
 Sample : N3358-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/21/2022

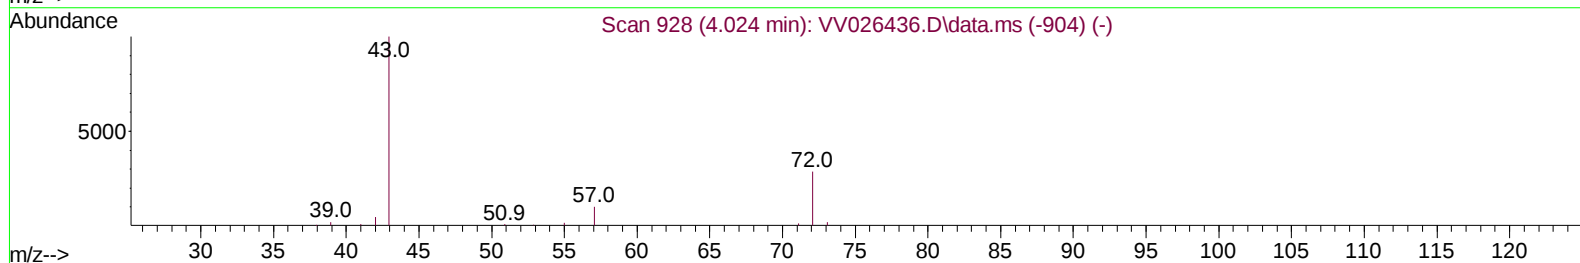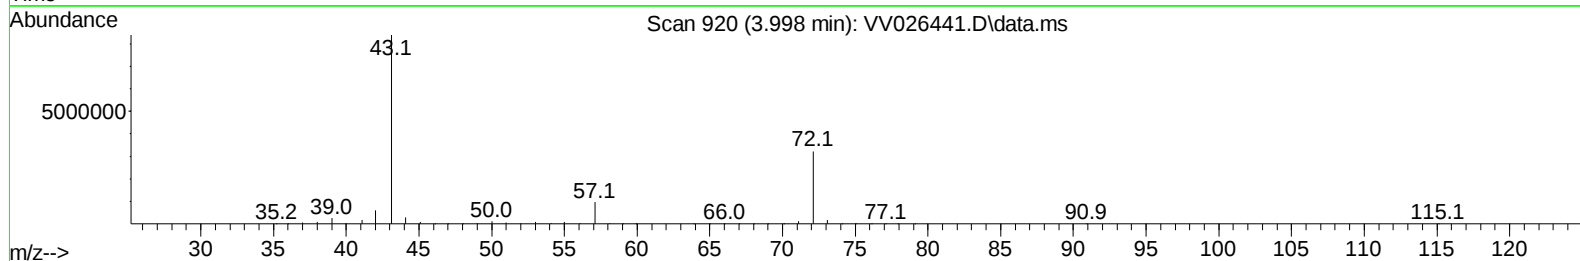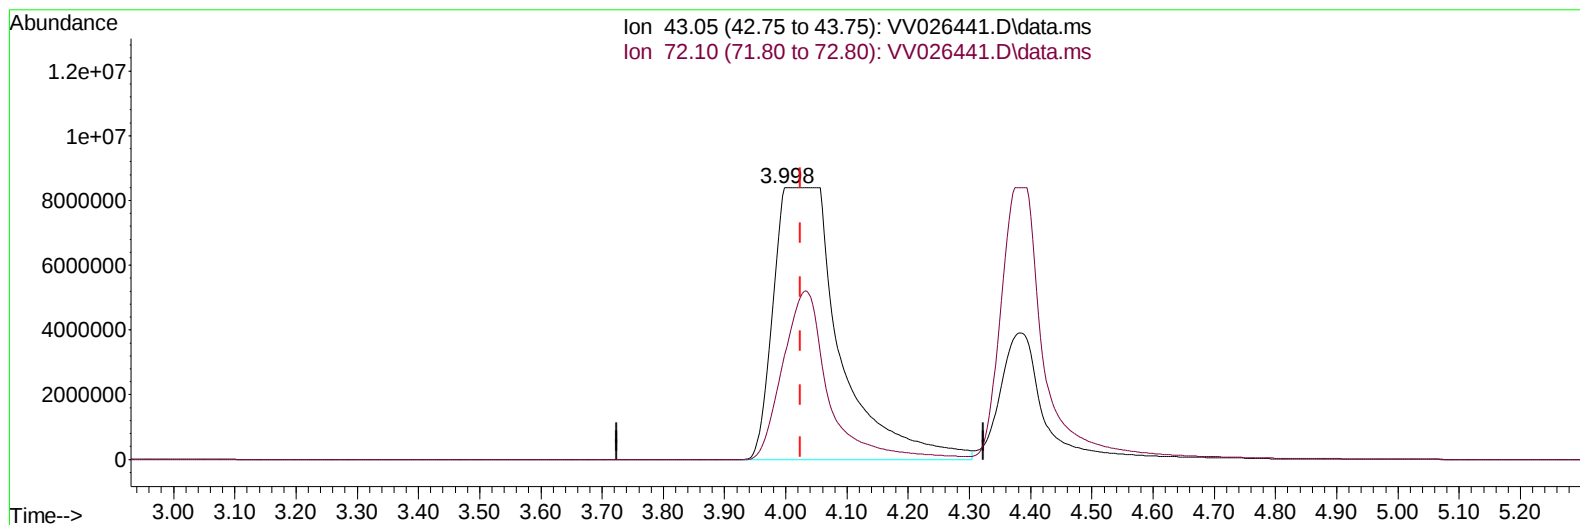

TIC: VV026441.D\data.ms

(21) 2-Butanone (T)

3.998min (-0.026) 31941.66 ug/L m

response 63261795

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026441.D
 Acq On : 20 Jun 2022 13:18
 Operator : SY/MD
 Sample : N3358-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/21/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.628	114		233042	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117		198440	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		90037	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.323	65		76961	3.802	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.000%	
7) Chloroethane-d5	1.587	69		64745	4.068	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.400%	
11) 1,1-Dichloroethene-d2	2.127	63		107737	3.100	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.000%	
20) 2-Butanone-d5	3.940	46		105801	53.568	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.140%	
24) Chloroform-d	4.410	84		140451	4.734	ug/L	0.05
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%	
26) 1,2-Dichloroethane-d4	5.053	65		53041	4.226	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.600%	
32) Benzene-d6	5.066	84		303331	5.718	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.400%	
36) 1,2-Dichloropropane-d6	6.079	67		80643	5.208	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.200%	
41) Toluene-d8	7.320	98		253240	5.235	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.600%	
43) trans-1,3-Dichloroprop...	7.632	79		14596	2.907	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.200%	
46) 2-Hexanone-d5	8.095	63		70094	46.215	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.440%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		47829	5.014	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152		80937	5.836	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.800%	
Target Compounds							
13) Acetone	2.224	43	28468100	18598.945	ug/L		Qvalue 85
14) Carbon disulfide	2.314	76	9032	0.249	ug/L		99
21) 2-Butanone	3.998	43	63261795m	31941.655	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026441.D
Acq On : 20 Jun 2022 13:18
Operator : SY/MD
Sample : N3358-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:33:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 02:31:12 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
Supervised By :Mahesh Dadoda 06/21/2022

