




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026444.D
 Acq On : 20 Jun 2022 14:29
 Operator : SY/MD
 Sample : N3355-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C7

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:34:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/21/2022

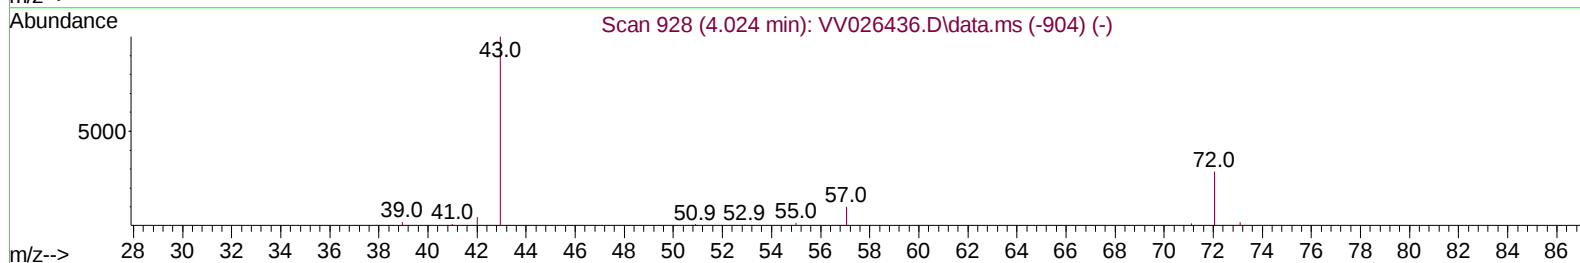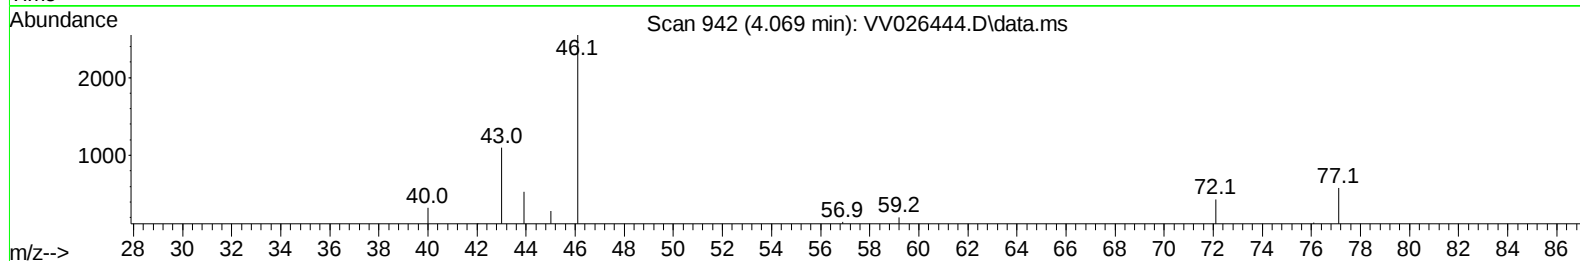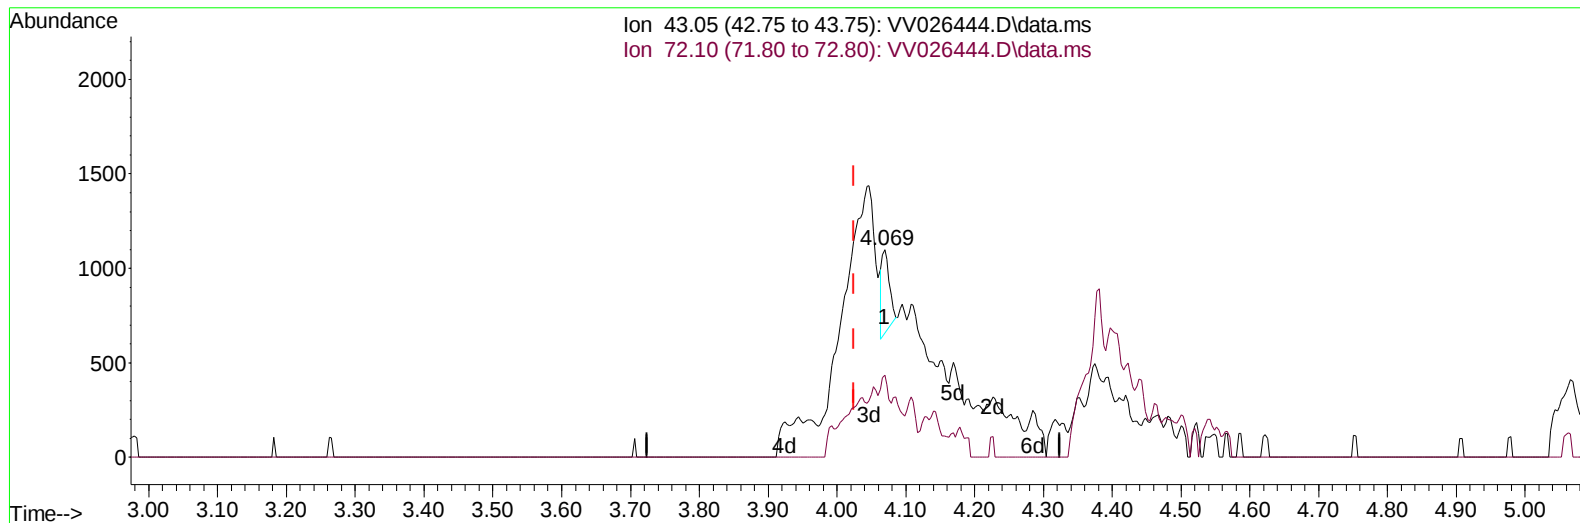

TIC: VV026444.D\data.ms

(21) 2-Butanone (T)

4.069min (+ 0.045) 0.19 ug/L

response 340

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	36.47
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026444.D
 Acq On : 20 Jun 2022 14:29
 Operator : SY/MD
 Sample : N3355-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C7

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:34:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/21/2022

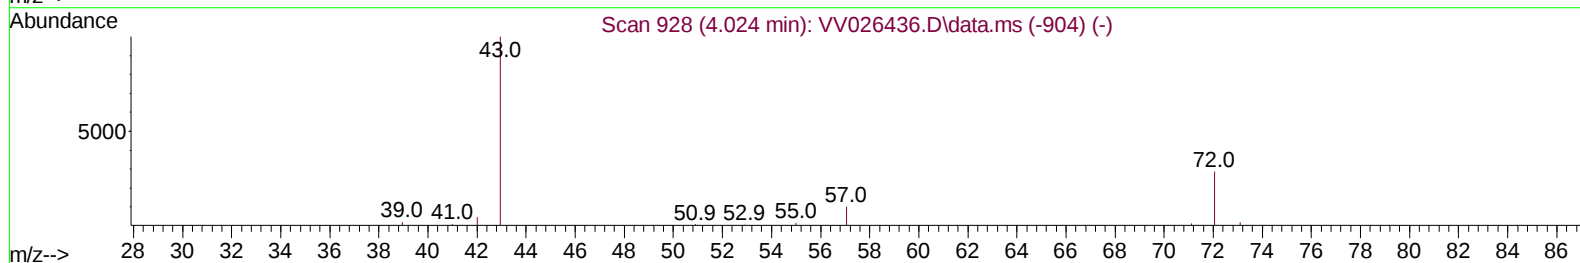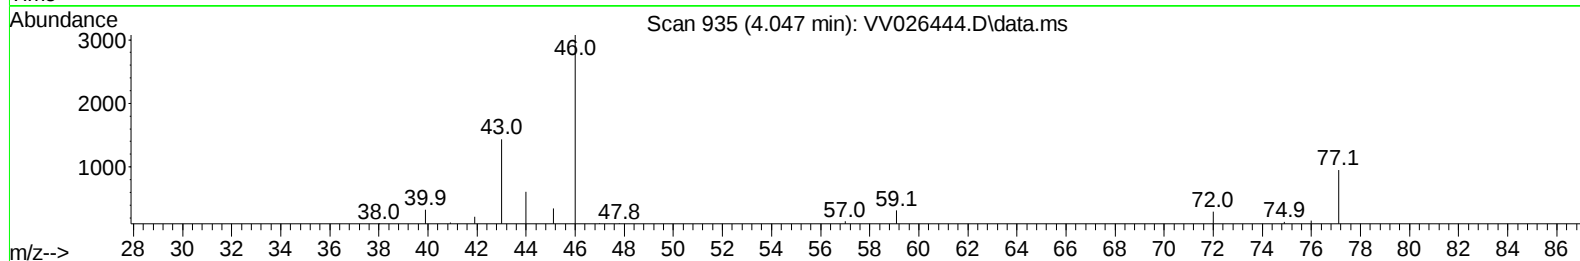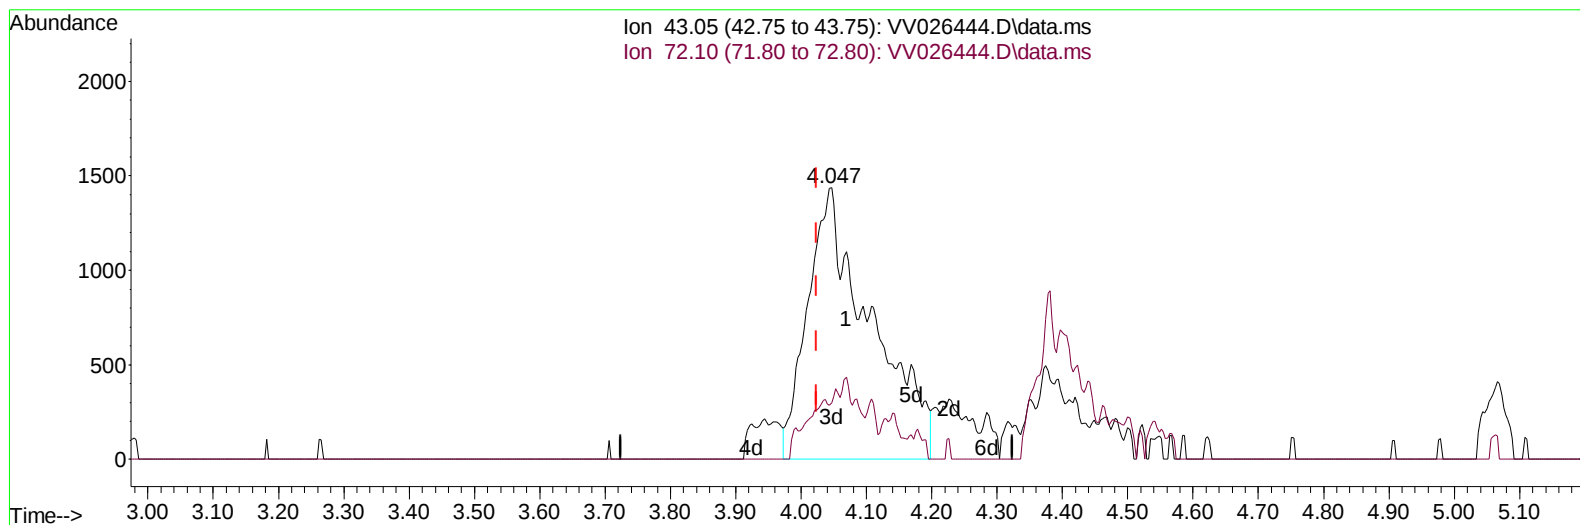

TIC: VV026444.D\data.ms

(21) 2-Butanone (T)

4.047min (+ 0.023) 5.32 ug/L m

response 9619

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	1.29#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026444.D
 Acq On : 20 Jun 2022 14:29
 Operator : SY/MD
 Sample : N3355-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C7

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:34:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/21/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	212838	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	193106	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79114	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	82896	4.484	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	89.600%		
7) Chloroethane-d5	1.587	69	70892	4.877	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	97.600%		
11) 1,1-Dichloroethene-d2	2.124	63	118089	3.720	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	74.400%		
20) 2-Butanone-d5	3.934	46	87624	48.576	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	97.160%		
24) Chloroform-d	4.365	84	151416	5.588	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	111.800%		
26) 1,2-Dichloroethane-d4	5.047	65	60272	5.258	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	105.200%		
32) Benzene-d6	5.063	84	315068	6.103	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	122.000%		
36) 1,2-Dichloropropane-d6	6.079	67	89438	5.936	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	118.800%		
41) Toluene-d8	7.320	98	266215	5.655	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	113.200%		
43) trans-1,3-Dichloroprop...	7.632	79	16838	3.446	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	69.000%		
46) 2-Hexanone-d5	8.095	63	69864	47.336	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	94.680%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49634	5.347	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	107.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	79244	6.503	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	130.000%#		
Target Compounds						
21) 2-Butanone	4.047	43	9619m	5.318	ug/L	
34) Trichloroethene	5.924	95	19820	1.466	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026444.D
Acq On : 20 Jun 2022 14:29
Operator : SY/MD
Sample : N3355-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/21/2022
Supervised By :Mahesh Dadoda 06/21/2022

Quant Time: Jun 21 02:34:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 02:31:12 2022
Response via : Initial Calibration

