




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026460.D
 Acq On : 20 Jun 2022 21:01
 Operator : SY/MD
 Sample : N3355-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C4

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:40:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

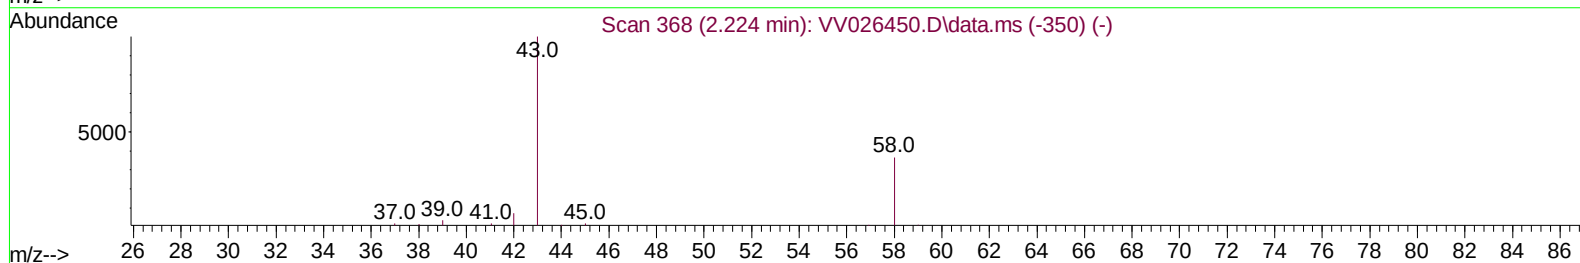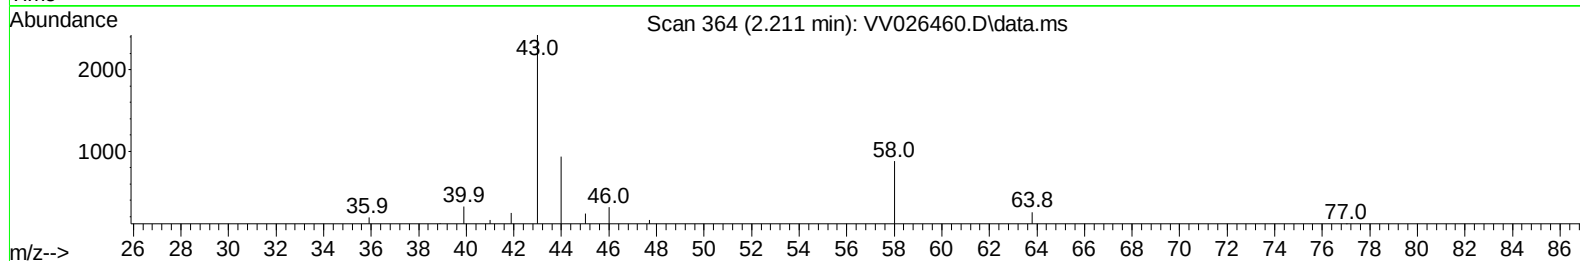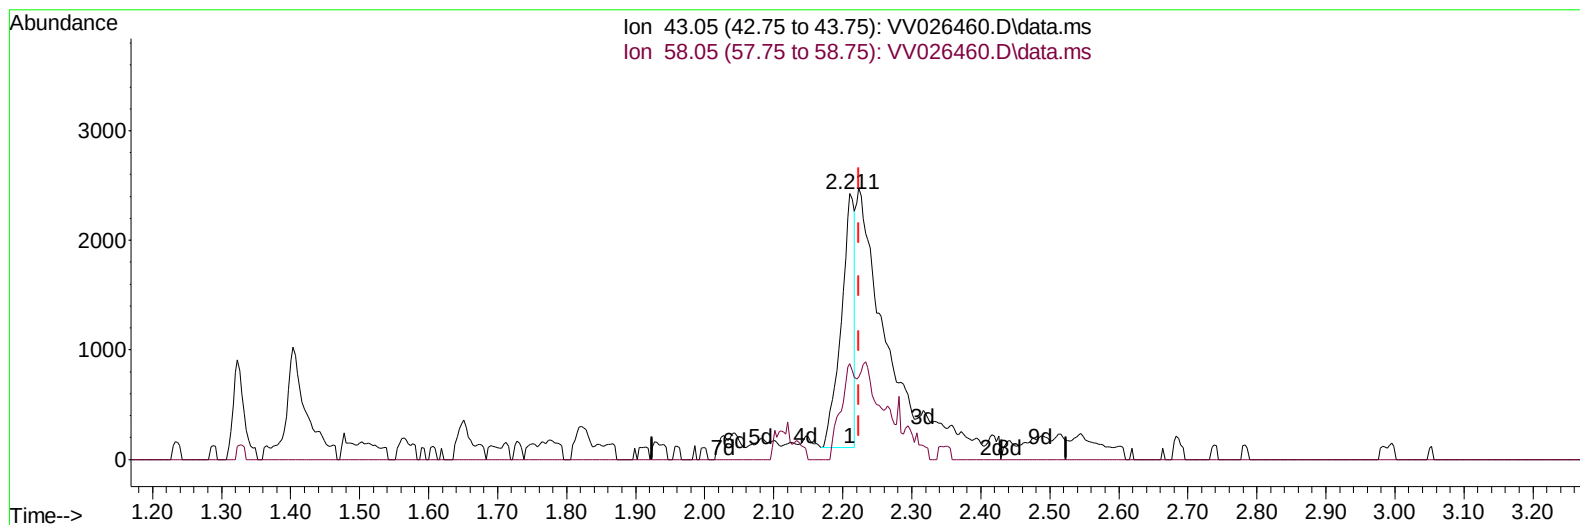

TIC: VV026460.D\data.ms

(13) Acetone (T)

2.211min (-0.013) 2.14 ug/L

response 3162

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	42.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026460.D
 Acq On : 20 Jun 2022 21:01
 Operator : SY/MD
 Sample : N3355-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C4

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:40:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

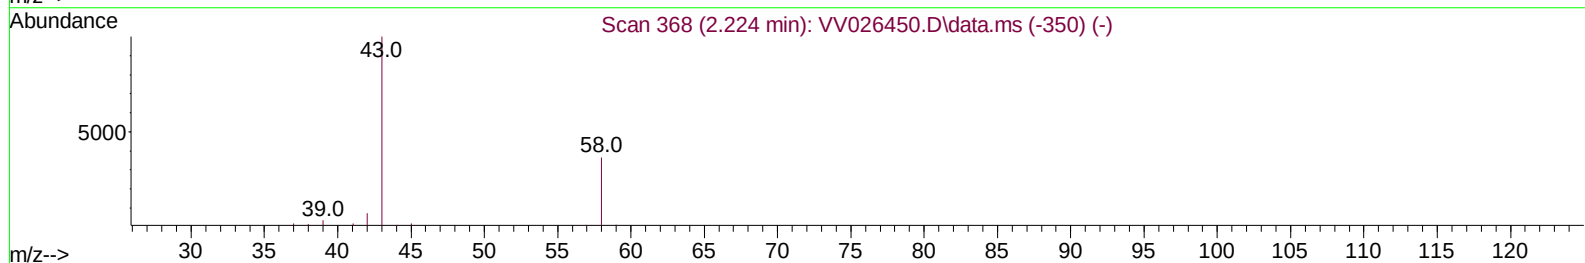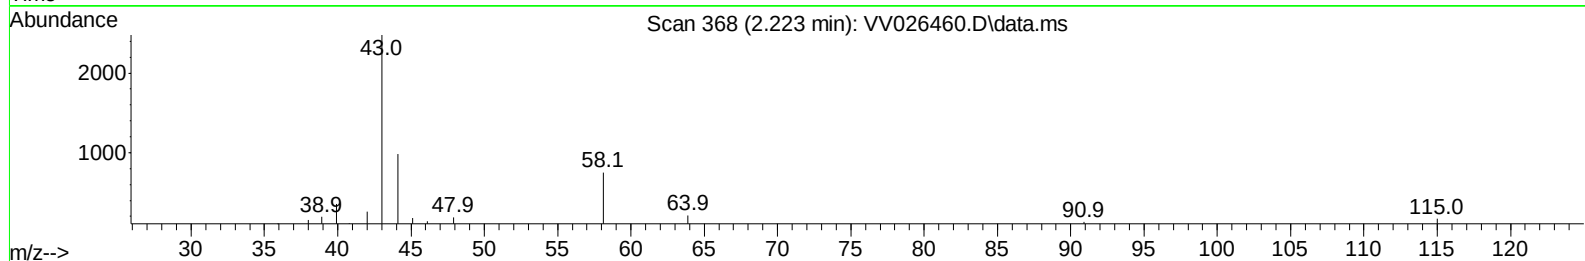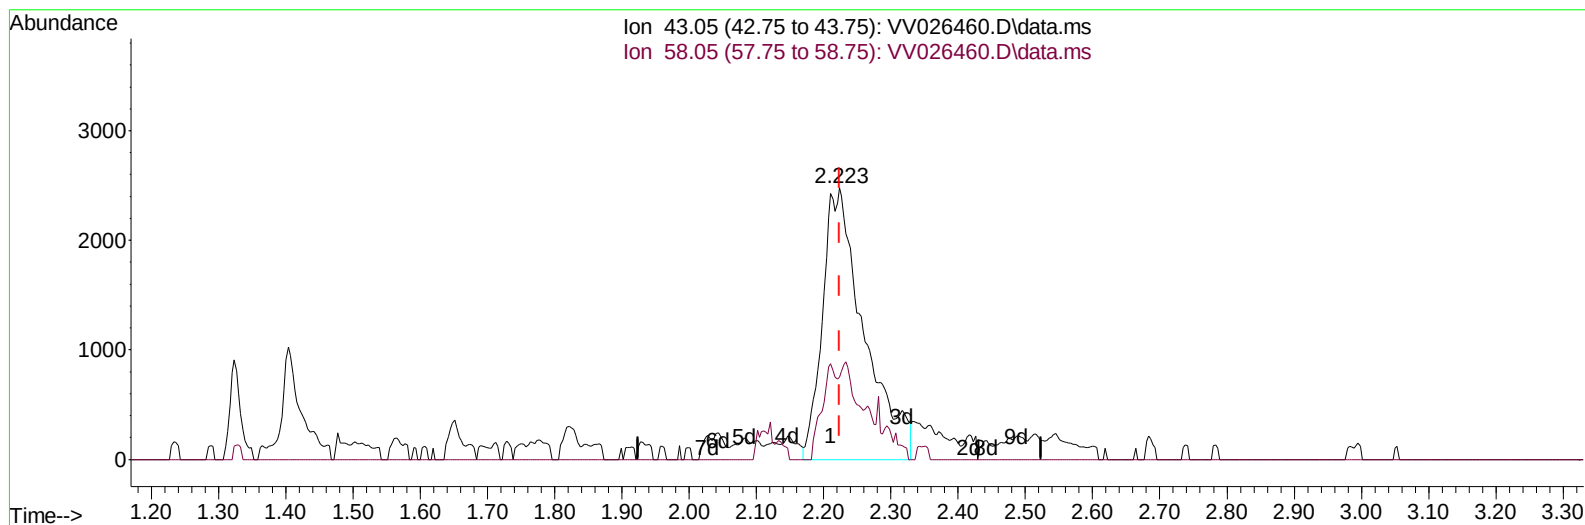

TIC: VV026460.D\data.ms

(13) Acetone (T)

2.223min (-0.000) 7.18 ug/L m

response 10603

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	12.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026460.D
 Acq On : 20 Jun 2022 21:01
 Operator : SY/MD
 Sample : N3355-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C4

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:40:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.625	114		224905	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117		201904	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		87313	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.323	65		79872	4.089	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.800%	
7) Chloroethane-d5	1.584	69		68806	4.480	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.600%	
11) 1,1-Dichloroethene-d2	2.124	63		115522	3.444	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.800%	
20) 2-Butanone-d5	3.924	46		101175	53.079	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.160%	
24) Chloroform-d	4.365	84		152786	5.336	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.800%	
26) 1,2-Dichloroethane-d4	5.043	65		62949	5.197	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%	
32) Benzene-d6	5.063	84		314235	5.821	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.400%	
36) 1,2-Dichloropropane-d6	6.075	67		89661	5.691	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.800%	
41) Toluene-d8	7.320	98		269932	5.484	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.600%	
43) trans-1,3-Dichloroprop...	7.628	79		16072	3.146	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.000%	
46) 2-Hexanone-d5	8.091	63		81305	52.687	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.380%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		53626	5.526	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152		83680	6.222	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	124.400%#	
Target Compounds							
13) Acetone	2.223	43		10603m	7.178	ug/L	
63) 1,2,4-Trimethylbenzene	10.914	105		19451	0.532	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026460.D
Acq On : 20 Jun 2022 21:01
Operator : SY/MD
Sample : N3355-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C4

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:40:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
Supervised By :Mahesh Dadoda 06/24/2022

