




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026462.D
Acq On : 20 Jun 2022 21:48
Operator : SY/MD
Sample : N3355-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D2

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/21/2022
Supervised By :Mahesh Dadoda 06/24/2022

Quant Time: Jun 21 05:41:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

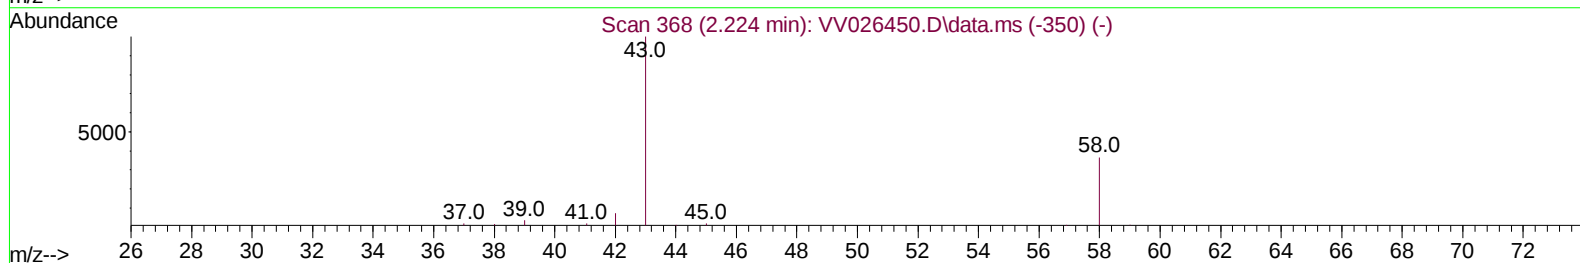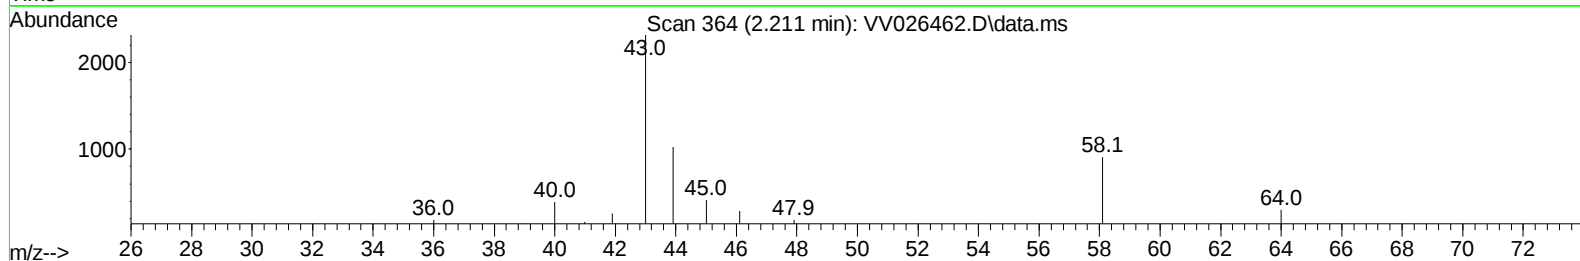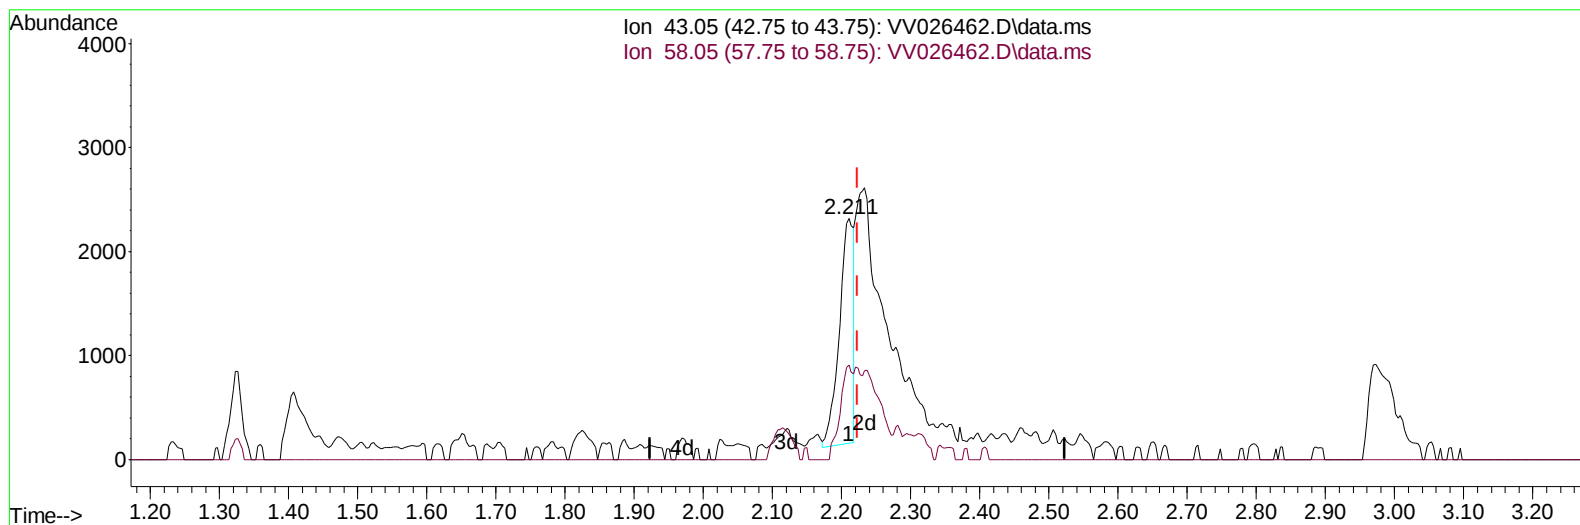

TIC: VV026462.D\data.ms

(13) Acetone (T)

2.211min (-0.013) 3.45 ug/L

response 3074

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	38.94
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026462.D
 Acq On : 20 Jun 2022 21:48
 Operator : SY/MD
 Sample : N3355-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D2

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

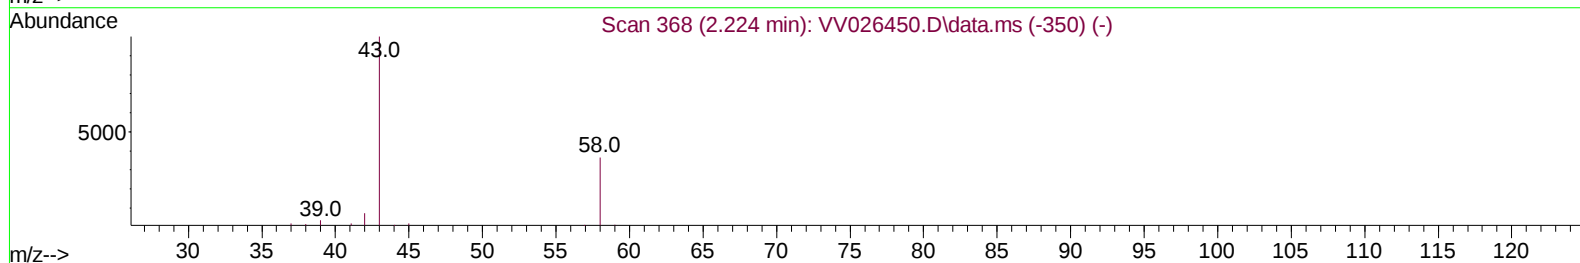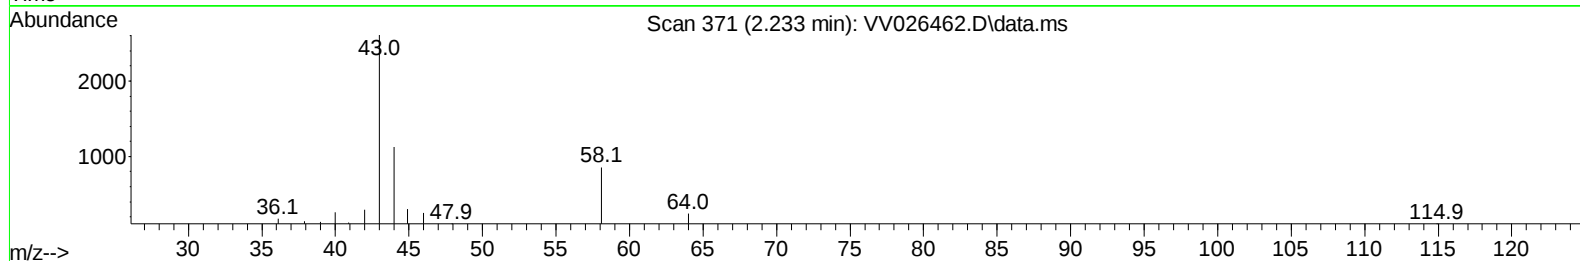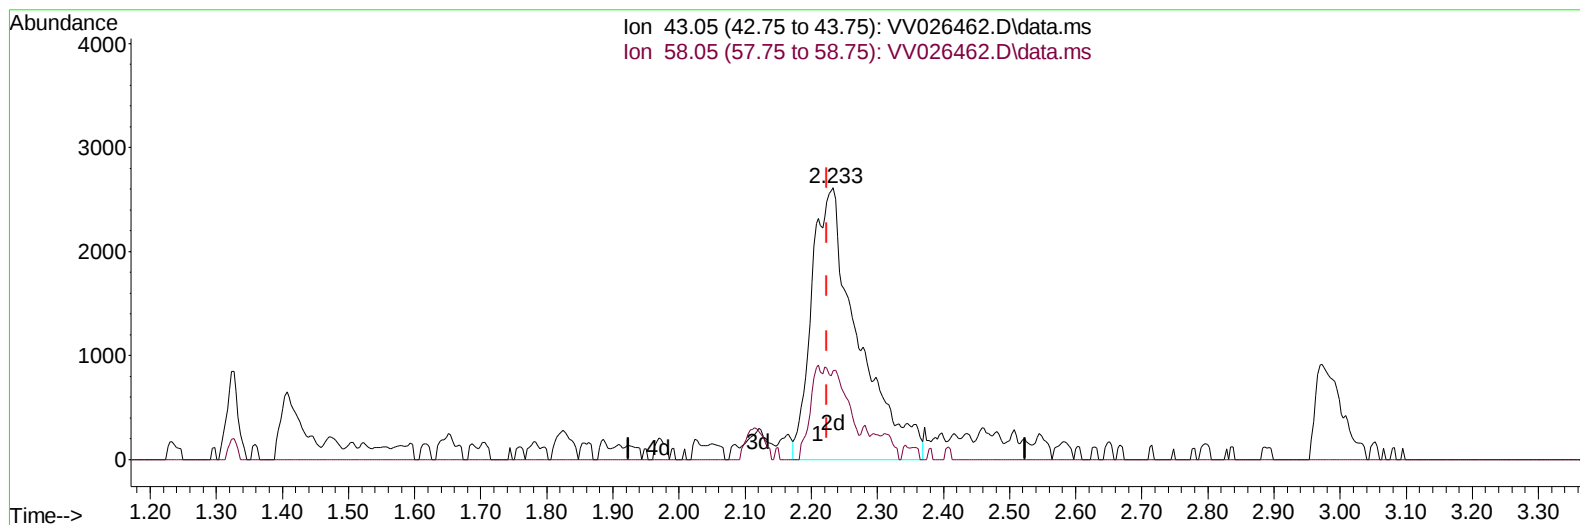

TIC: VV026462.D\data.ms

(13) Acetone (T)

2.233min (+ 0.009) 14.25 ug/L m

response 12685

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	9.44
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026462.D
 Acq On : 20 Jun 2022 21:48
 Operator : SY/MD
 Sample : N3355-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D2

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.628	114	135517	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	122345	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50666	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	69069	5.868	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	117.400%	
7) Chloroethane-d5	1.584	69	61178	6.610	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	132.200%#	
11) 1,1-Dichloroethene-d2	2.124	63	96268	4.763	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	95.200%	
20) 2-Butanone-d5	3.928	46	90965	79.201	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	158.400%#	
24) Chloroform-d	4.365	84	131082	7.598	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	152.000%#	
26) 1,2-Dichloroethane-d4	5.047	65	54736	7.499	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	150.000%#	
32) Benzene-d6	5.063	84	255912	7.824	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	156.400%#	
36) 1,2-Dichloropropane-d6	6.079	67	76441	8.007	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	160.200%#	
41) Toluene-d8	7.320	98	206750	6.932	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	138.600%#	
43) trans-1,3-Dichloroprop...	7.632	79	13719	4.432	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	88.600%	
46) 2-Hexanone-d5	8.095	63	69616	74.449	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	148.900%#	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46964	7.986	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	159.800%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	64118	8.216	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	164.400%#	
Target Compounds						
3) Chloromethane	1.259	50	5154	0.458	ug/L	92
13) Acetone	2.233	43	12685m	14.252	ug/L	
63) 1,2,4-Trimethylbenzene	10.918	105	3303	0.156	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026462.D
Acq On : 20 Jun 2022 21:48
Operator : SY/MD
Sample : N3355-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D2

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
Supervised By :Mahesh Dadoda 06/24/2022

