




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026463.D
 Acq On : 20 Jun 2022 22:12
 Operator : SY/MD
 Sample : N3355-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D3

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

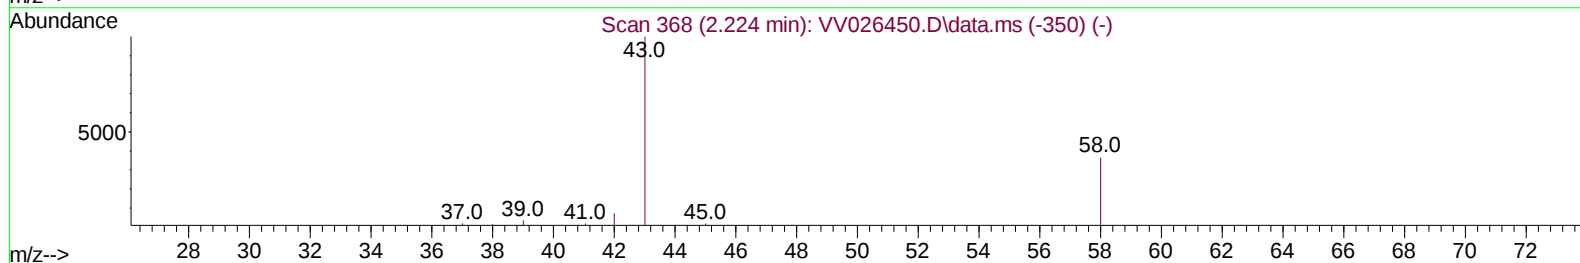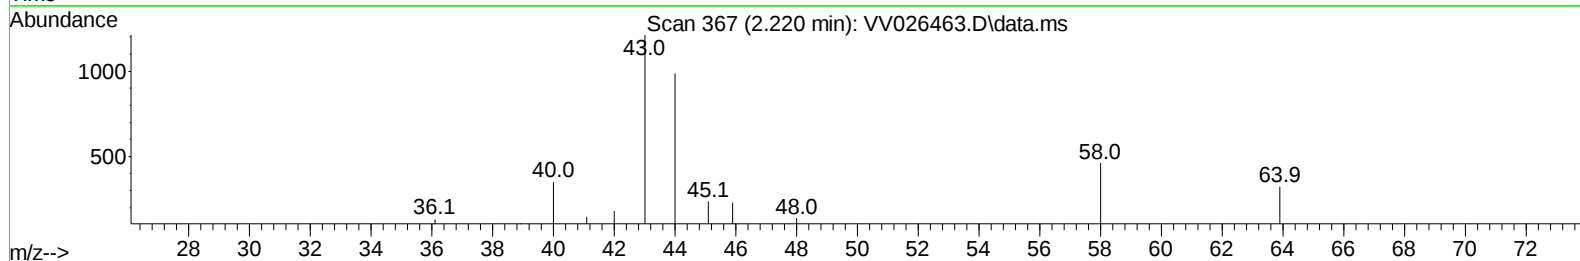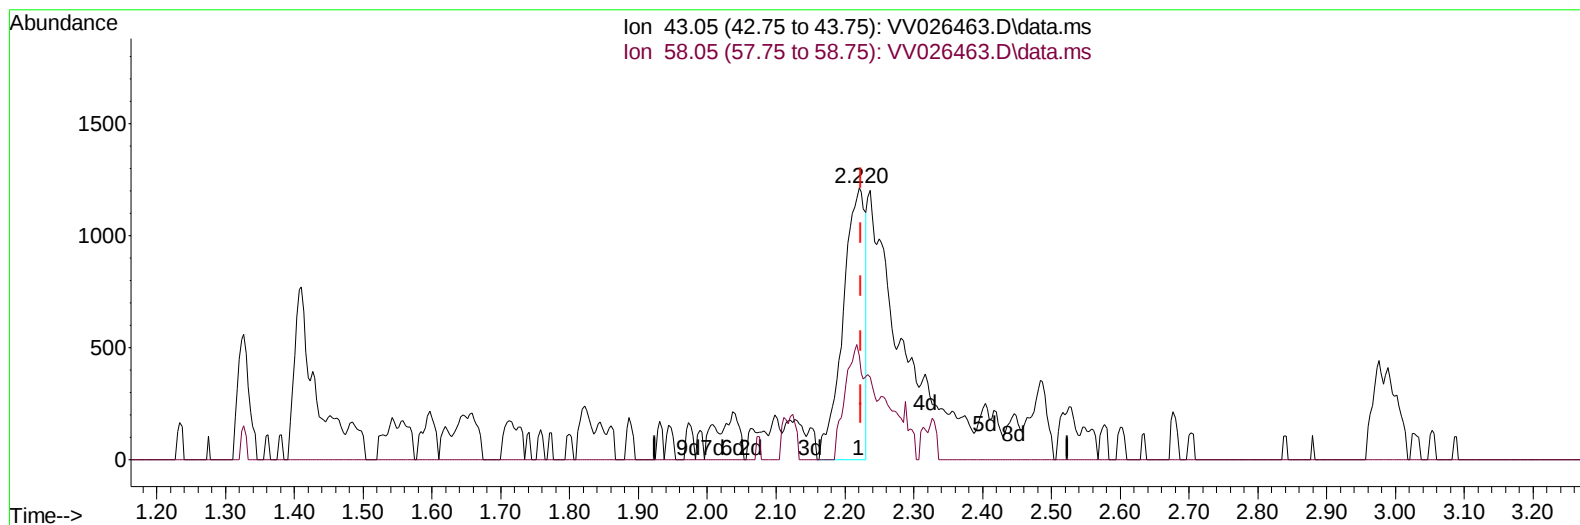

TIC: VV026463.D\data.ms

(13) Acetone (T)

2.220min (-0.003) 2.21 ug/L

response 2704

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	32.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026463.D
 Acq On : 20 Jun 2022 22:12
 Operator : SY/MD
 Sample : N3355-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D3

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

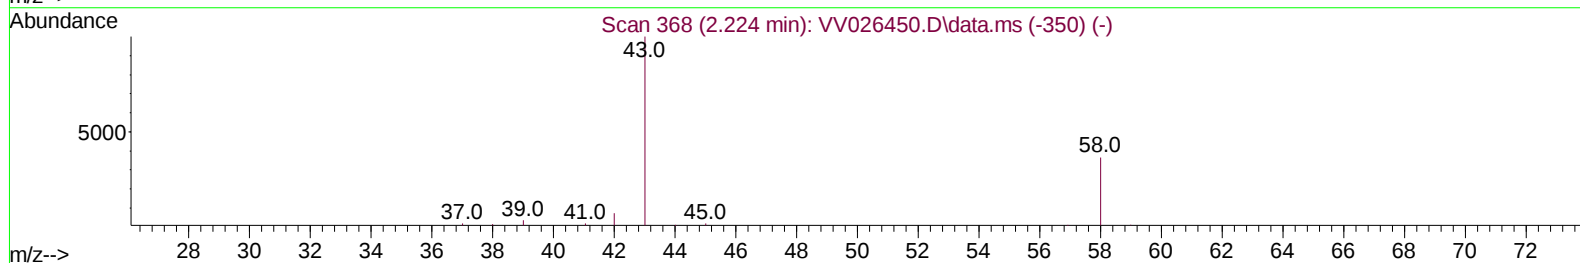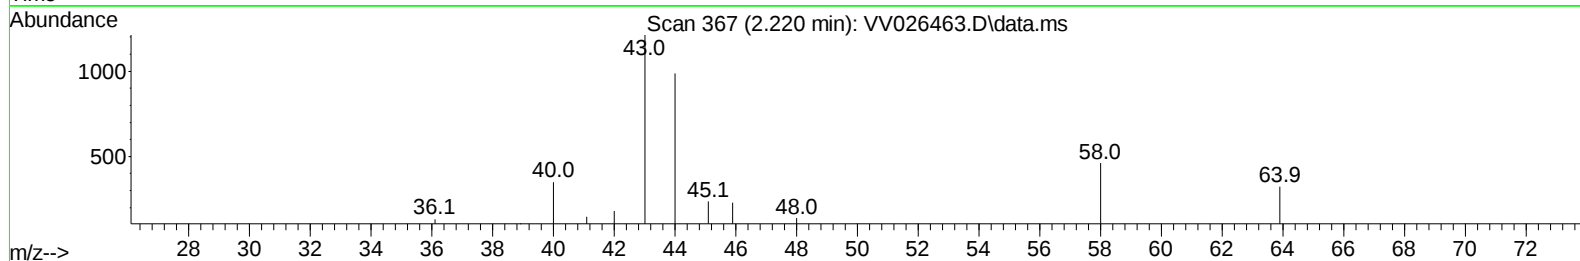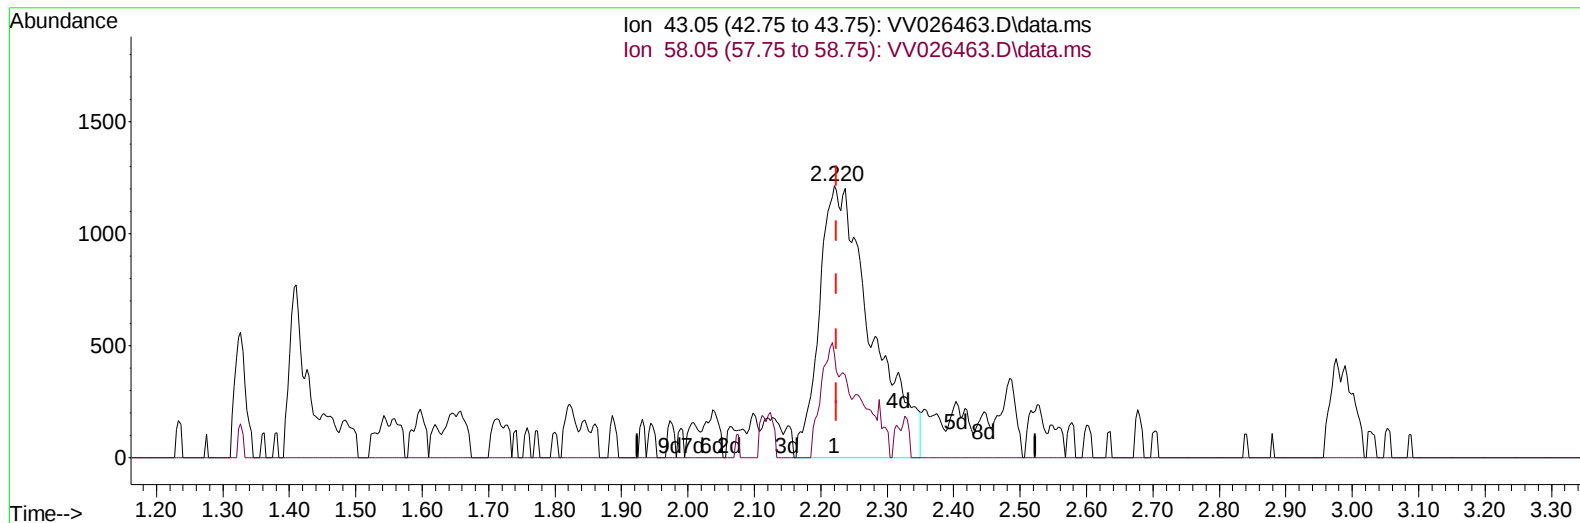

TIC: VV026463.D\data.ms

(13) Acetone (T)

2.220min (-0.003) 5.40 ug/L m

response 6607

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	13.27
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026463.D
 Acq On : 20 Jun 2022 22:12
 Operator : SY/MD
 Sample : N3355-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D3

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	186121	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	171046	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71852	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	73377	4.539	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	90.800%	
7) Chloroethane-d5	1.584	69	65086	5.120	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	102.400%	
11) 1,1-Dichloroethene-d2	2.124	63	107221	3.862	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	77.200%	
20) 2-Butanone-d5	3.931	46	87530	55.490	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	110.980%	
24) Chloroform-d	4.362	84	134536	5.678	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	113.600%	
26) 1,2-Dichloroethane-d4	5.043	65	57130	5.699	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	114.000%	
32) Benzene-d6	5.063	84	278427	6.089	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	121.800%	
36) 1,2-Dichloropropane-d6	6.079	67	83812	6.280	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	125.600%	
41) Toluene-d8	7.320	98	237671	5.700	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	114.000%	
43) trans-1,3-Dichloroprop...	7.632	79	15240	3.521	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	70.400%	
46) 2-Hexanone-d5	8.095	63	72331	55.328	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	110.660%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	51023	6.206	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	124.200%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	72943	6.591	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	131.800%#	
Target Compounds						
						Qvalue
3) Chloromethane	1.259	50	3667	0.237	ug/L	94
13) Acetone	2.220	43	6607m	5.405	ug/L	
22) cis-1,2-Dichloroethene	3.937	96	1561	0.135	ug/L	92
34) Trichloroethene	5.918	95	478780	39.991	ug/L	99
47) Tetrachloroethene	7.989	164	449	0.051	ug/L	82
63) 1,2,4-Trimethylbenzene	10.921	105	2081	0.069	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026463.D
Acq On : 20 Jun 2022 22:12
Operator : SY/MD
Sample : N3355-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D3

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
Supervised By :Mahesh Dadoda 06/24/2022

