




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026464.D
 Acq On : 20 Jun 2022 22:36
 Operator : SY/MD
 Sample : N3355-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C5

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

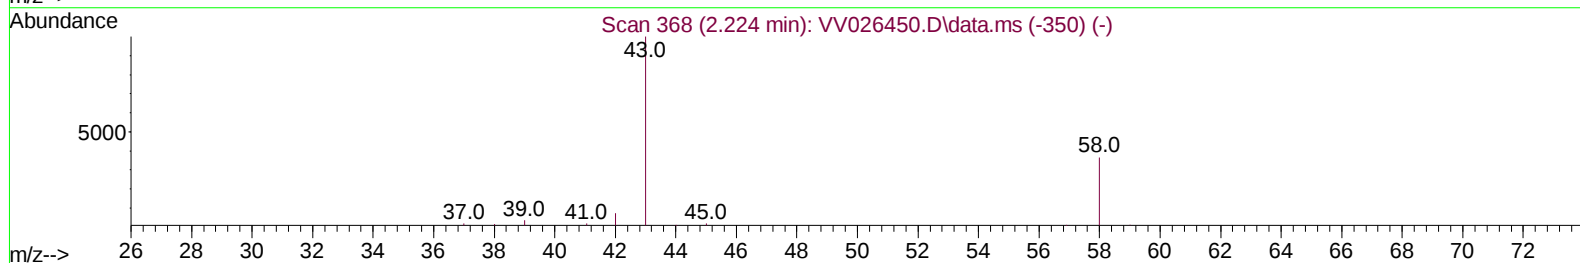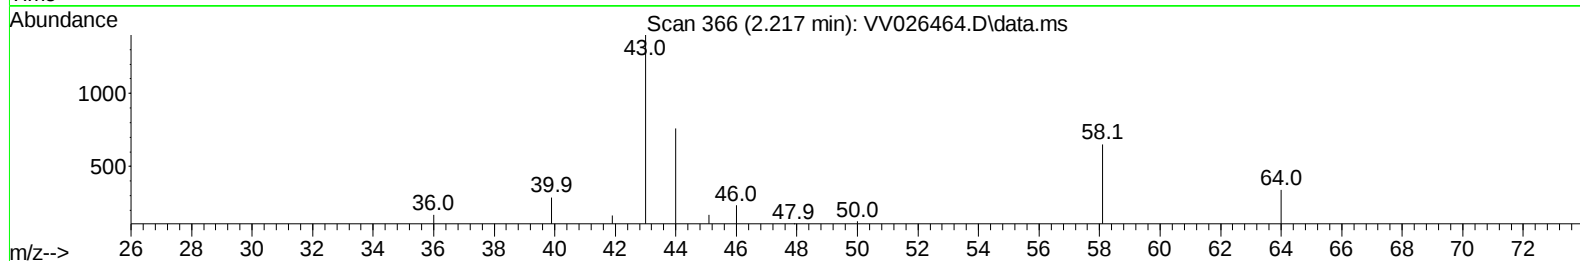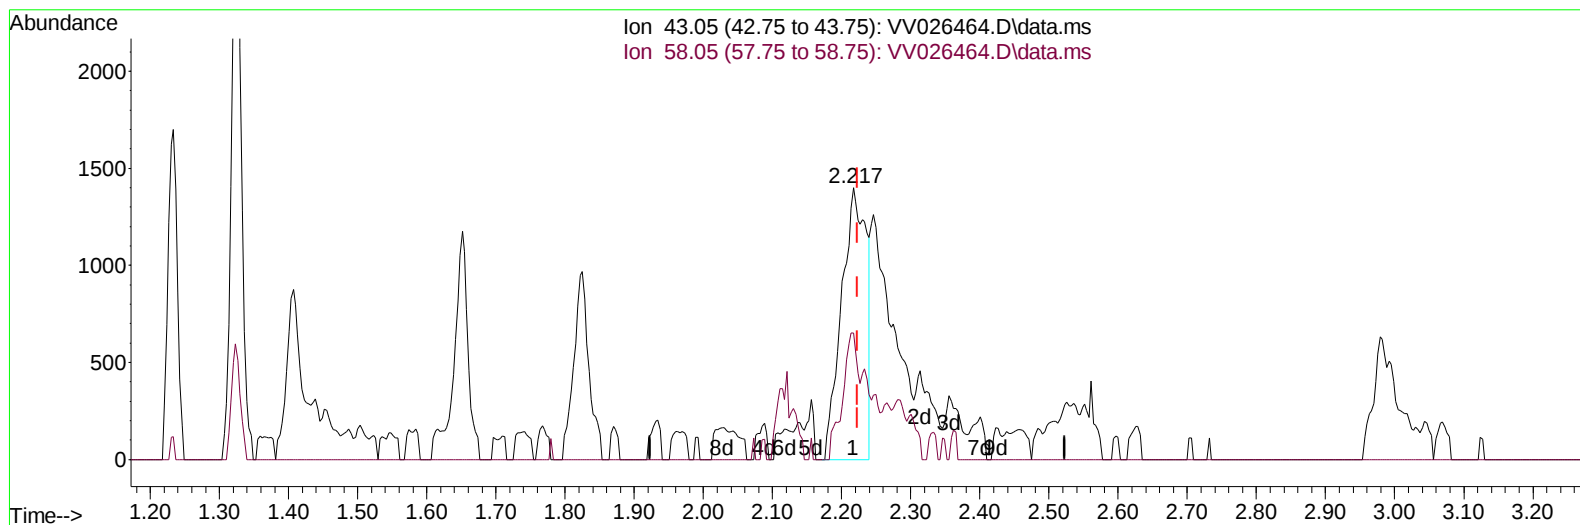

TIC: VV026464.D\data.ms

(13) Acetone (T)

2.217min (-0.007) 2.75 ug/L

response 3475

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	29.73
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026464.D
 Acq On : 20 Jun 2022 22:36
 Operator : SY/MD
 Sample : N3355-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C5

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

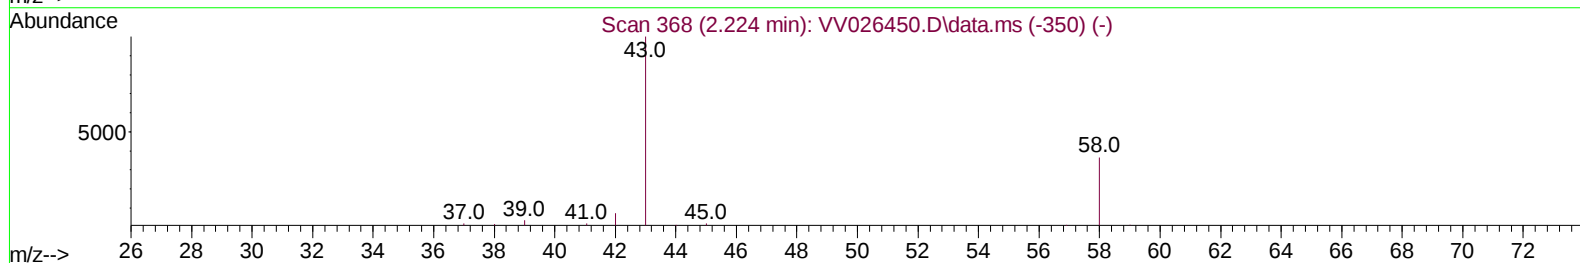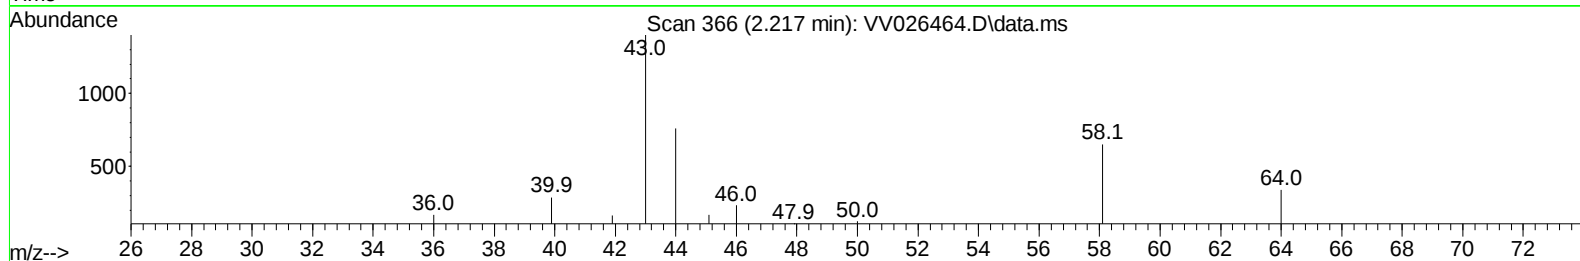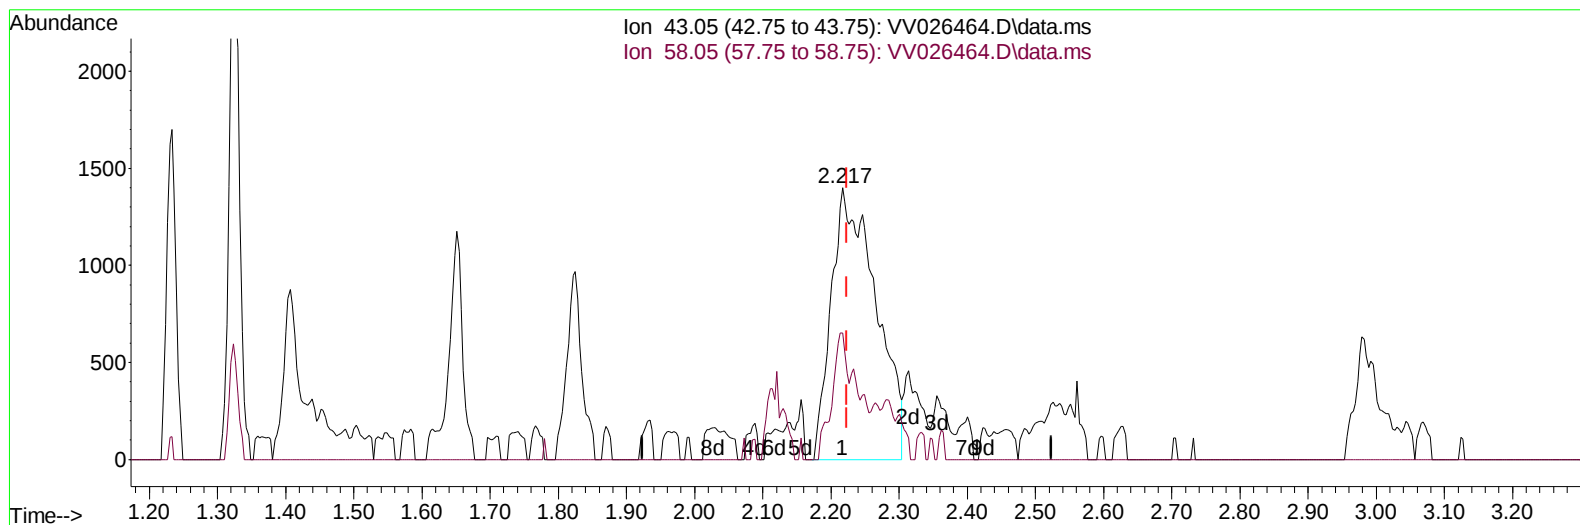

TIC: VV026464.D\data.ms

(13) Acetone (T)

2.217min (-0.007) 5.02 ug/L m

response 6344

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	16.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026464.D
 Acq On : 20 Jun 2022 22:36
 Operator : SY/MD
 Sample : N3355-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C5

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	192357	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	177928	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68534	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	68274	4.086	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	81.800%	
7) Chloroethane-d5	1.584	69	59261	4.511	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.200%	
11) 1,1-Dichloroethene-d2	2.124	63	96109	3.350	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.000%	
20) 2-Butanone-d5	3.931	46	89700	55.022	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	110.040%	
24) Chloroform-d	4.365	84	127728	5.216	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.400%	
26) 1,2-Dichloroethane-d4	5.047	65	52775	5.094	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.800%	
32) Benzene-d6	5.063	84	258667	5.438	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	108.800%	
36) 1,2-Dichloropropane-d6	6.079	67	76853	5.536	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	110.800%	
41) Toluene-d8	7.320	98	214297	4.941	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.800%	
43) trans-1,3-Dichloroprop...	7.632	79	14001	3.110	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	62.200%	
46) 2-Hexanone-d5	8.095	63	65739	48.341	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.680%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47515	5.556	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	111.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	64020	6.065	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	121.200%#	
Target Compounds						
3) Chloromethane	1.259	50	5144	0.322	ug/L	88
13) Acetone	2.217	43	6344m	5.021	ug/L	
63) 1,2,4-Trimethylbenzene	10.921	105	1891	0.066	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026464.D
Acq On : 20 Jun 2022 22:36
Operator : SY/MD
Sample : N3355-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C5

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:41:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
Supervised By :Mahesh Dadoda 06/24/2022

