




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026471.D
 Acq On : 21 Jun 2022 01:23
 Operator : SY/MD
 Sample : N3345-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:43:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

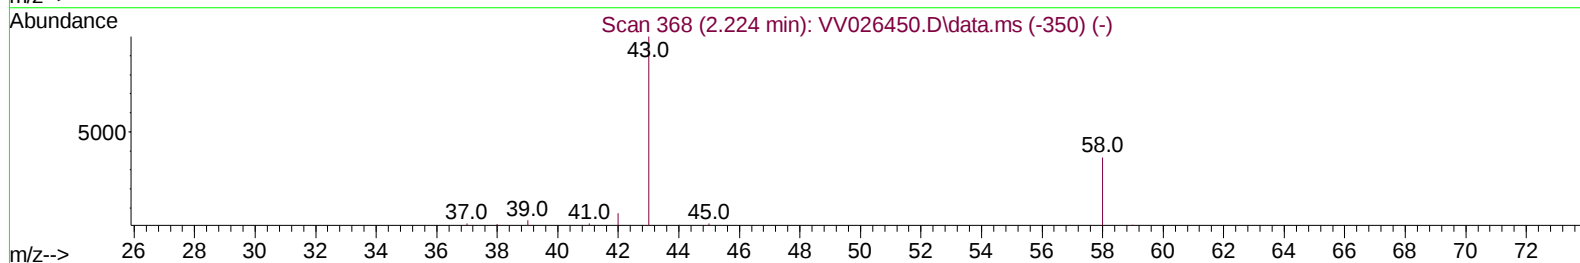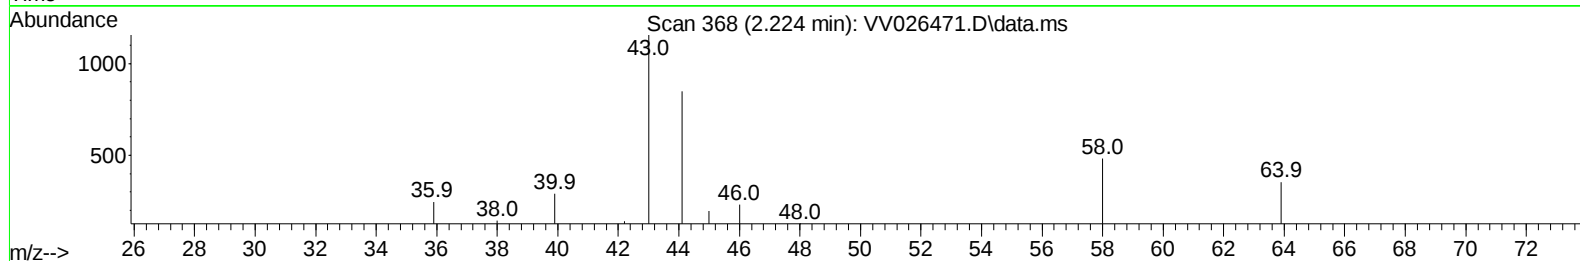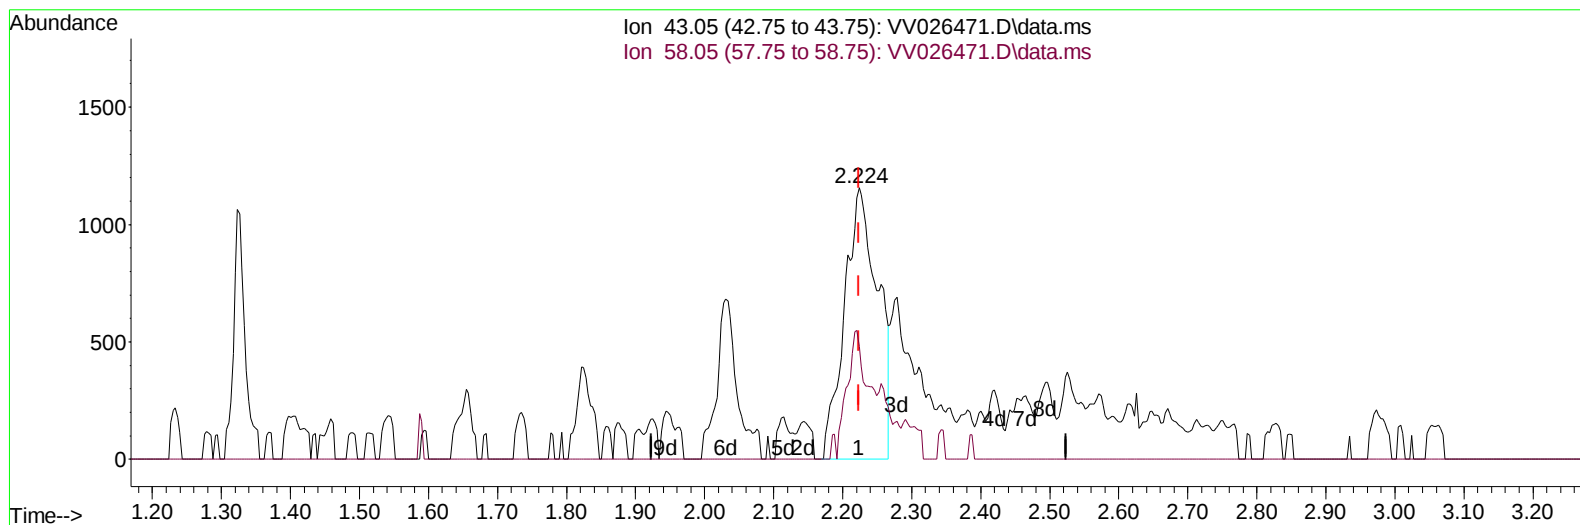

TIC: VV026471.D\data.ms

(13) Acetone (T)

2.224min (0.000) 3.26 ug/L

response 3844

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	30.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026471.D
 Acq On : 21 Jun 2022 01:23
 Operator : SY/MD
 Sample : N3345-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:43:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

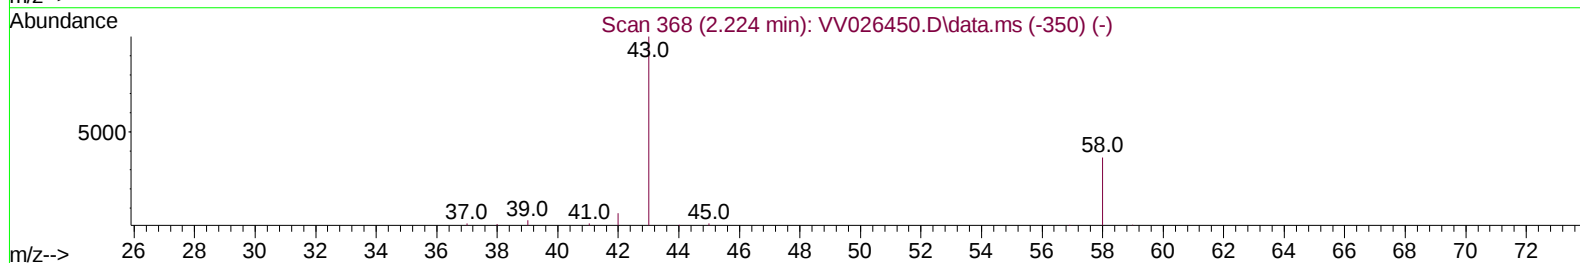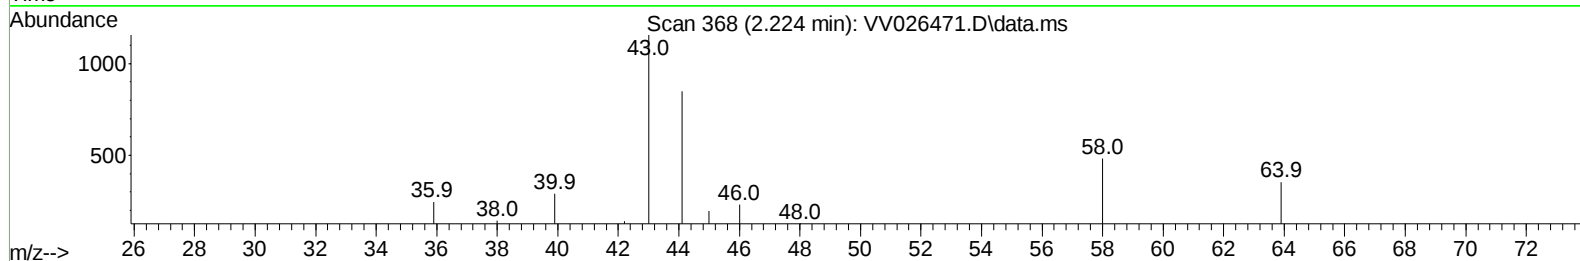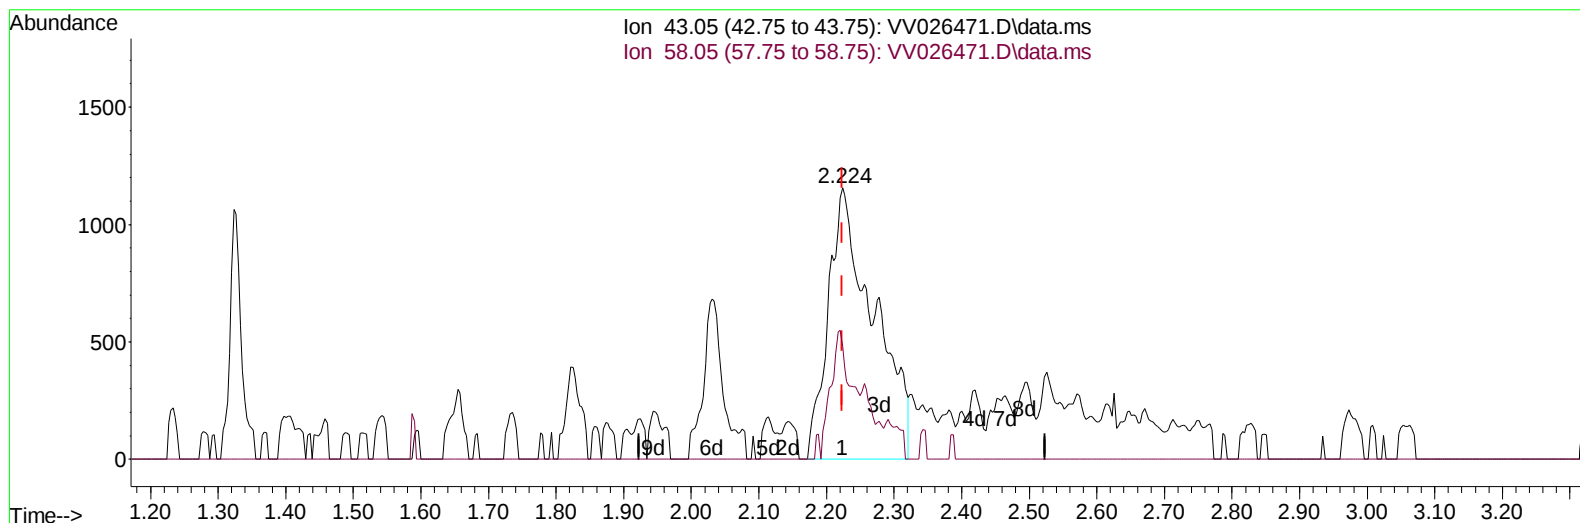

TIC: VV026471.D\data.ms

(13) Acetone (T)

2.224min (0.000) 4.57 ug/L m

response 5381

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	21.76
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026471.D
 Acq On : 21 Jun 2022 01:23
 Operator : SY/MD
 Sample : N3345-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:43:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
 Supervised By :Mahesh Dadoda 06/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	179349	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	169411	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69953	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	60404	3.878	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	77.600%	
7) Chloroethane-d5	1.587	69	54436	4.444	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	88.800%	
11) 1,1-Dichloroethene-d2	2.124	63	89169	3.333	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	66.600%	
20) 2-Butanone-d5	3.928	46	91804	60.397	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	120.800%	
24) Chloroform-d	4.365	84	122459	5.363	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	107.200%	
26) 1,2-Dichloroethane-d4	5.047	65	49425	5.117	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	102.400%	
32) Benzene-d6	5.063	84	233879	5.164	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.200%	
36) 1,2-Dichloropropane-d6	6.076	67	70614	5.342	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	106.800%	
41) Toluene-d8	7.320	98	192508	4.661	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	93.200%	
43) trans-1,3-Dichloroprop...	7.629	79	15714	3.666	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	73.400%	
46) 2-Hexanone-d5	8.092	63	65156	50.321	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	100.640%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	44816	5.504	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	110.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	62023	5.756	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	115.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.224	43	5381m	4.568	ug/L	
14) Carbon disulfide	2.310	76	9070	0.325	ug/L	100
22) cis-1,2-Dichloroethene	3.934	96	5986	0.538	ug/L	86
25) Chloroform	4.394	83	55680	2.449	ug/L	99
33) Benzene	5.121	78	2908	0.067	ug/L	100
34) Trichloroethene	5.931	95	5536	0.467	ug/L	95
38) Bromodichloromethane	6.523	83	821	0.060	ug/L #	80
42) Toluene	7.400	91	10403	0.228	ug/L	99
47) Tetrachloroethene	7.979	164	18888	2.150	ug/L	99
53) m,p-Xylene	9.156	106	1241	0.070	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026471.D
Acq On : 21 Jun 2022 01:23
Operator : SY/MD
Sample : N3345-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 05:43:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/21/2022
Supervised By :Mahesh Dadoda 06/24/2022

