

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062022\
 Data File : VW026439.D
 Acq On : 20 Jun 2022 12:30
 Operator : SY/MD
 Sample : N3358-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S4

Quant Time: Jun 21 02:32:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.629	114	228042	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	210142	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	86339	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.327	65	81718	4.126	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	82.600%	
7) Chloroethane-d5	1.587	69	70389	4.520	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.400%	
11) 1,1-Dichloroethene-d2	2.127	63	117169	3.445	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.800%	
20) 2-Butanone-d5	3.937	46	92521	47.871	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	95.740%	
24) Chloroform-d	4.368	84	151341	5.213	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.200%	
26) 1,2-Dichloroethane-d4	5.050	65	60614	4.935	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.800%	
32) Benzene-d6	5.063	84	311373	5.542	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.800%	
36) 1,2-Dichloropropane-d6	6.079	67	89487	5.458	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	109.200%	
41) Toluene-d8	7.320	98	263145	5.137	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.800%	
43) trans-1,3-Dichloroprop...	7.632	79	18991	3.572	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	71.400%	
46) 2-Hexanone-d5	8.095	63	73094	45.510	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.020%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	51911	5.139	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	102.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	80059	6.020	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	120.400%#	
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.314	76	22248	0.626	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026439.D
Acq On : 20 Jun 2022 12:30
Operator : SY/MD
Sample : N3358-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S4

Quant Time: Jun 21 02:32:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 02:31:12 2022
Response via : Initial Calibration

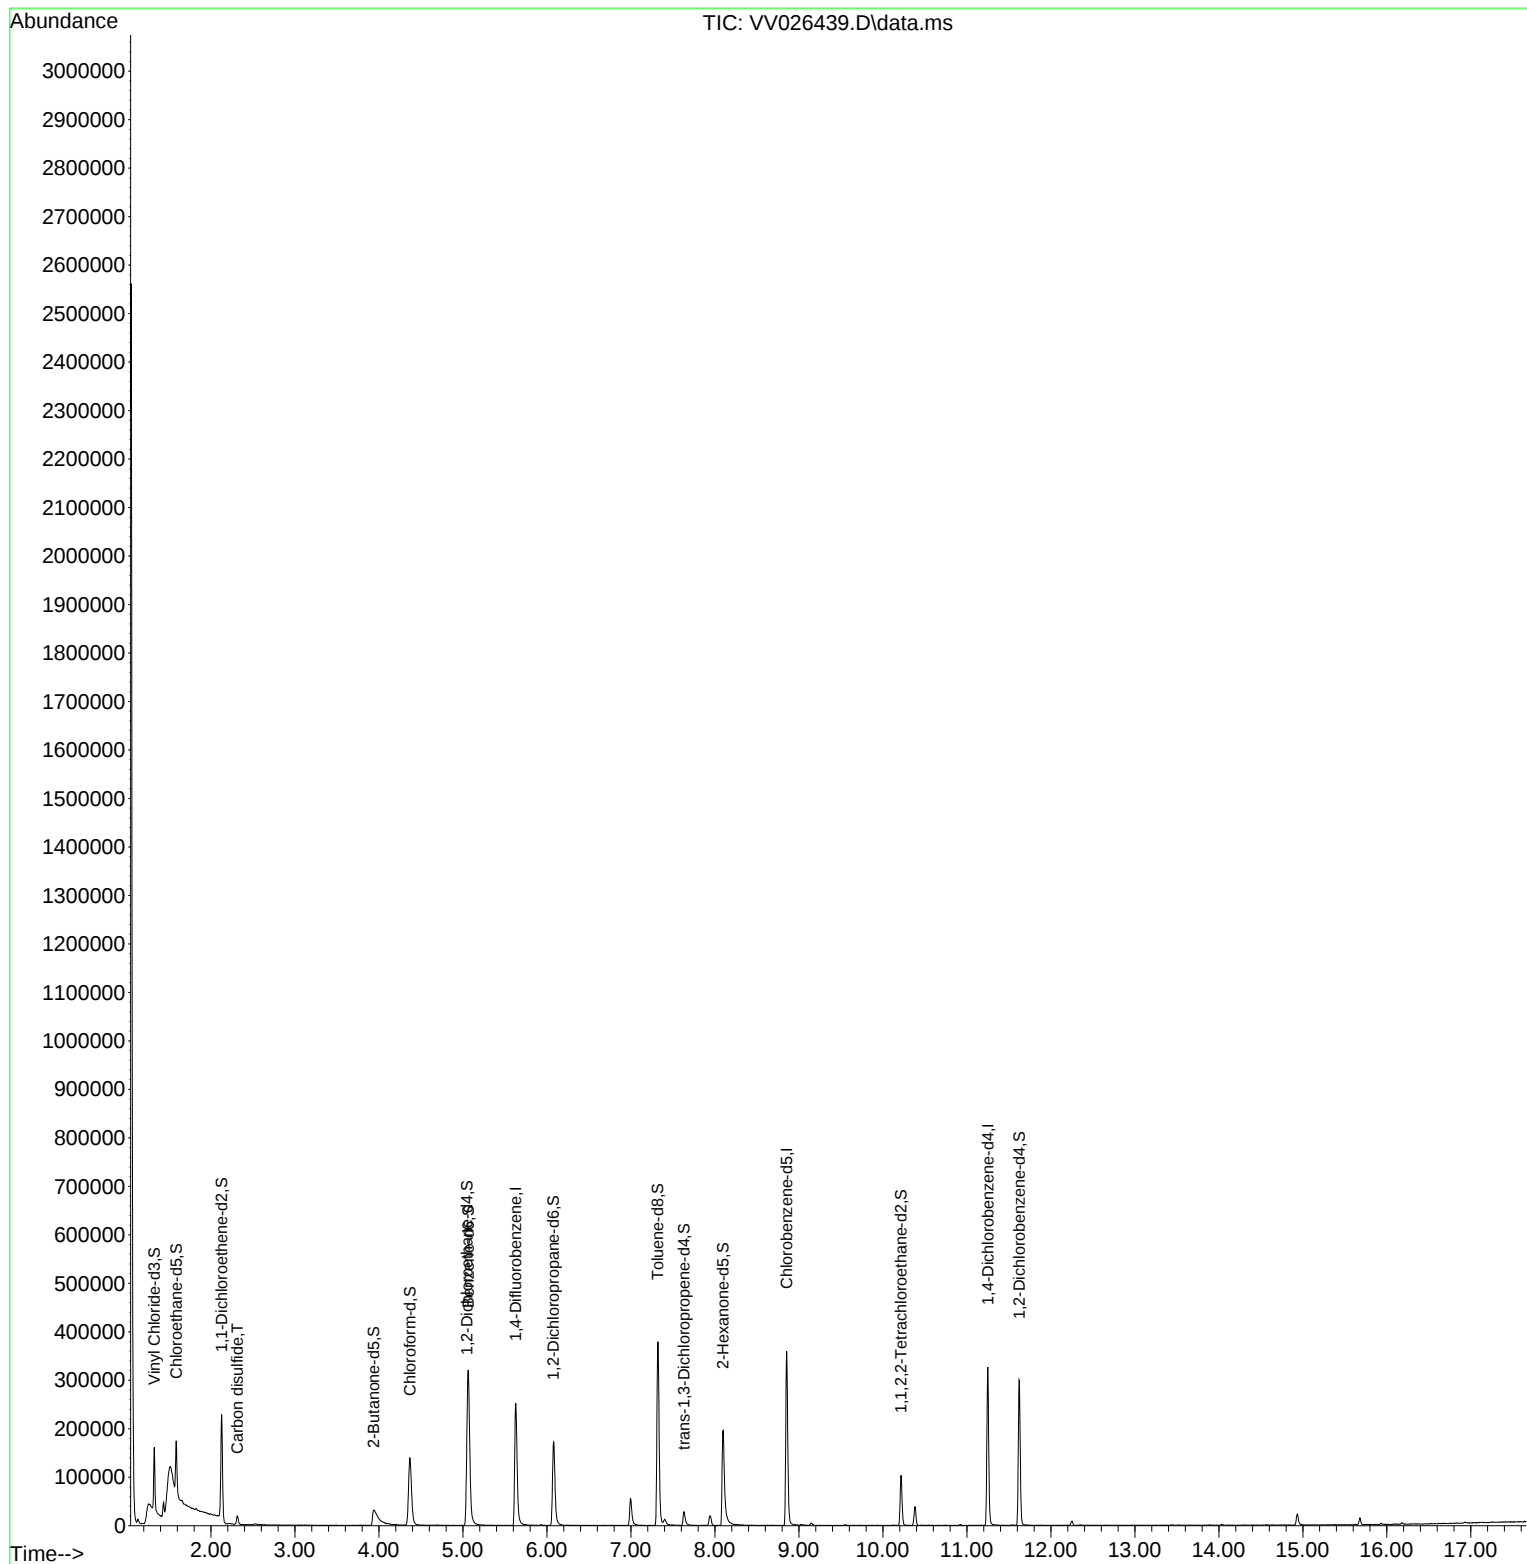

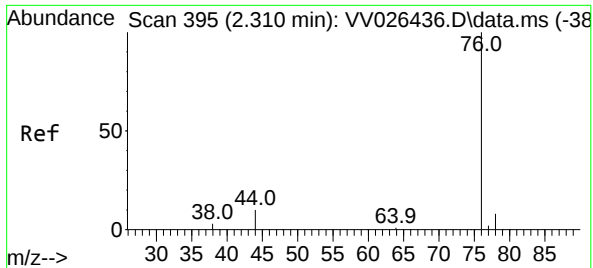

#14
Carbon disulfide
Concen: 0.626 ug/L
RT: 2.314 min Scan# 395
Delta R.T. 0.003 min
Lab File: VV026439.D
Acq: 20 Jun 2022 12:30

Instrument :
MSVOA_V
ClientSampleId :
EW4S4

Tgt Ion: 76 Resp: 22248
Ion Ratio Lower Upper
76 100
78 9.0 7.7 11.5

