

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062022\
 Data File : VW026442.D
 Acq On : 20 Jun 2022 13:42
 Operator : SY/MD
 Sample : N3358-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S9

Quant Time: Jun 21 02:33:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.629	114	230730	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	199617	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	92572	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	77876	3.886	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.800%	
7) Chloroethane-d5	1.587	69	65947	4.185	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.800%	
11) 1,1-Dichloroethene-d2	2.127	63	110178	3.201	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.000%	
20) 2-Butanone-d5	3.940	46	103969	53.168	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.340%	
24) Chloroform-d	4.378	84	146240	4.979	ug/L	0.02
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.600%	
26) 1,2-Dichloroethane-d4	5.050	65	55313	4.451	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.000%	
32) Benzene-d6	5.063	84	309605	5.801	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	116.000%	
36) 1,2-Dichloropropane-d6	6.079	67	82717	5.311	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.200%	
41) Toluene-d8	7.320	98	256686	5.275	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.400%	
43) trans-1,3-Dichloroprop...	7.632	79	16319	3.231	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	64.600%	
46) 2-Hexanone-d5	8.095	63	70584	46.264	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.520%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	48334	5.037	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	84172	5.903	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	118.000%	
Target Compounds						
13) Acetone	2.224	43	12113575	7993.414	ug/L	86
14) Carbon disulfide	2.310	76	7310	0.203	ug/L #	94
21) 2-Butanone	4.008	43	33277298	16970.479	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026442.D
Acq On : 20 Jun 2022 13:42
Operator : SY/MD
Sample : N3358-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S9

Quant Time: Jun 21 02:33:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 02:31:12 2022
Response via : Initial Calibration

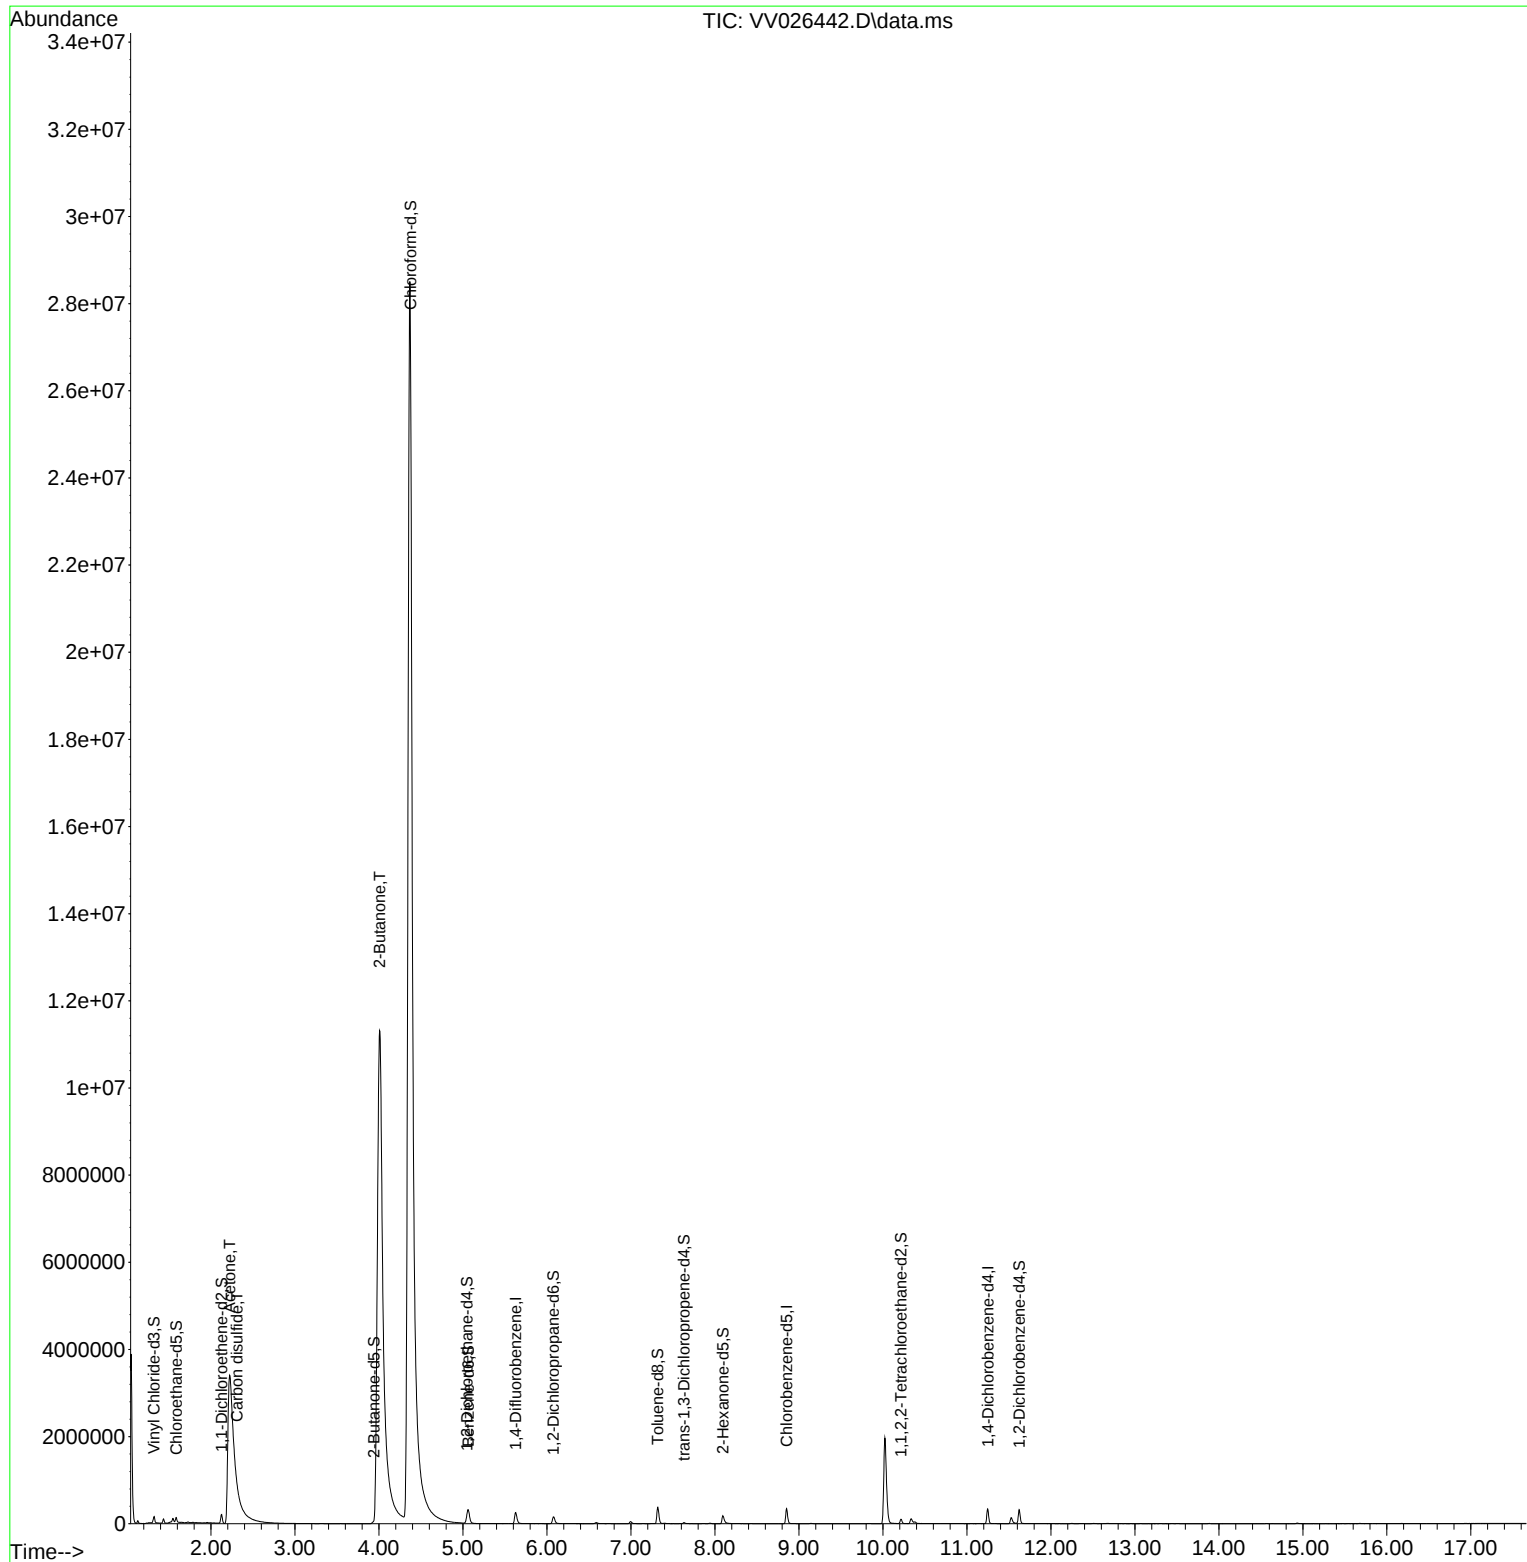

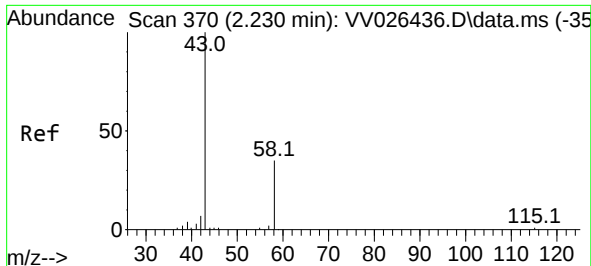

#13

Acetone

Concen: 7993.414 ug/L

RT: 2.224 min Scan# 3

Delta R.T. -0.006 min

Lab File: VV026442.D

Acq: 20 Jun 2022 13:42

Instrument :

MSVOA_V

ClientSampleId :





EW4S9

Tgt Ion: 43 Resp:12113575

Ion Ratio Lower Upper

43 100

58 37.3 0.0 60.0

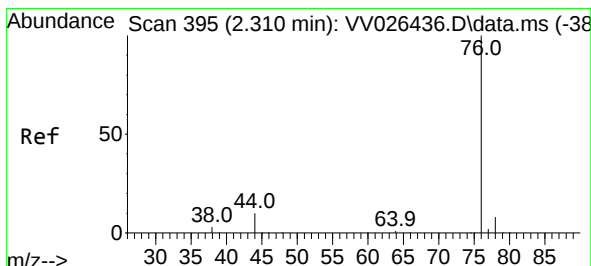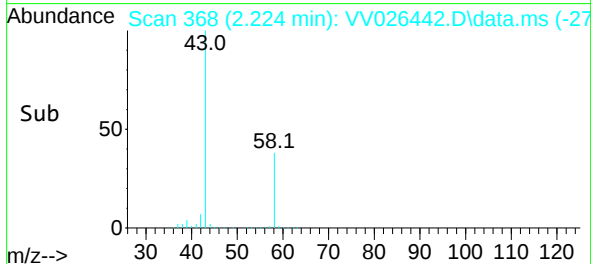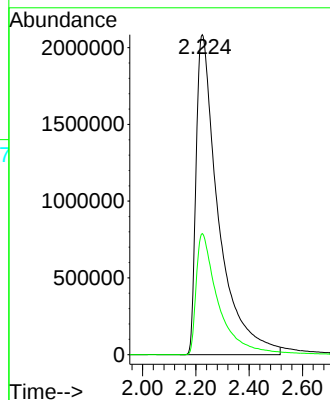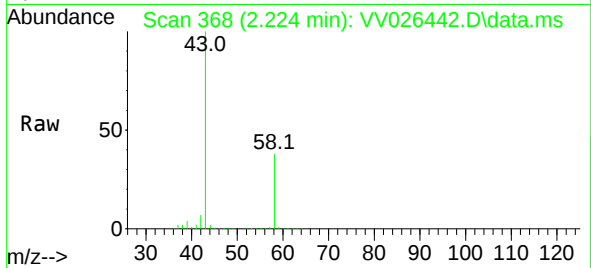

#14

Carbon disulfide

Concen: 0.203 ug/L

RT: 2.310 min Scan# 395

Delta R.T. -0.000 min

Lab File: VV026442.D




Acq: 20 Jun 2022 13:42


Tgt Ion: 76 Resp: 7310

Ion Ratio Lower Upper

76 100

78 11.9 7.7 11.5#

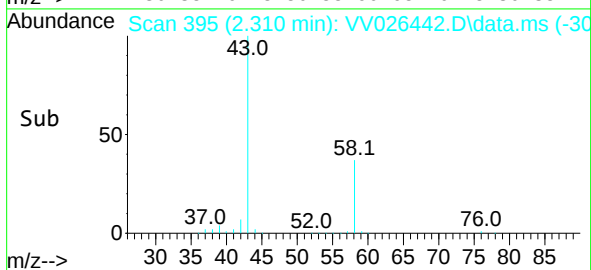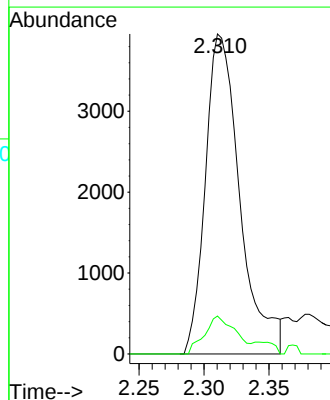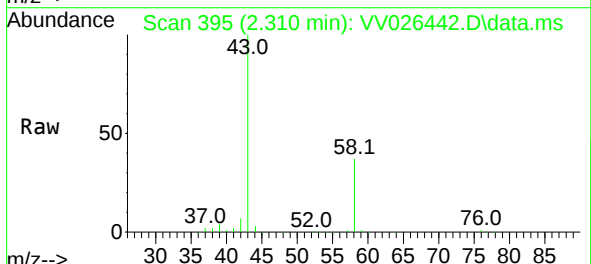

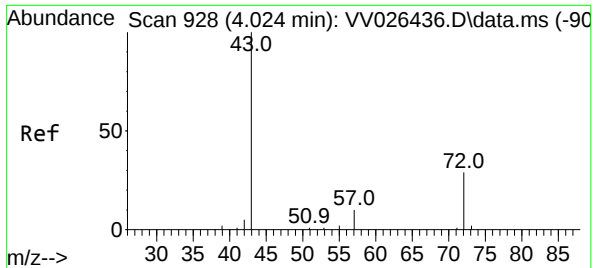

#21
2-Butanone
Concen: 16970.479 ug/L
RT: 4.008 min Scan# 91
Delta R.T. -0.016 min
Lab File: VV026442.D
Acq: 20 Jun 2022 13:42

Instrument :
MSVOA_V
ClientSampleId :
EW4S9

Tgt Ion: 43 Resp:33277298
Ion Ratio Lower Upper
43 100
72 33.1 12.7 38.0

