

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026448.D
 Acq On : 20 Jun 2022 16:12
 Operator : SY/MD
 Sample : N3256-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK3

Quant Time: Jun 21 02:35:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	194288	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	181400	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76438	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	71553	4.240	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.800%
7) Chloroethane-d5	1.587	69	61019	4.599	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.000%
11) 1,1-Dichloroethene-d2	2.124	63	103764	3.581	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.600%
20) 2-Butanone-d5	3.928	46	84191	51.129	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.260%
24) Chloroform-d	4.362	84	135276	5.469	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.400%
26) 1,2-Dichloroethane-d4	5.043	65	51903	4.960	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	5.059	84	267779	5.522	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.400%
36) 1,2-Dichloropropane-d6	6.075	67	78328	5.534	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.600%
41) Toluene-d8	7.317	98	224841	5.084	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
43) trans-1,3-Dichloroprop...	7.628	79	16714	3.642	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.800%
46) 2-Hexanone-d5	8.091	63	64689	46.658	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.320%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45168	5.180	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	69928	5.939	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.800%
Target Compounds						Qvalue
16) Methylene chloride	2.526	84	7019	0.448	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026448.D
Acq On : 20 Jun 2022 16:12
Operator : SY/MD
Sample : N3256-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK3


Quant Time: Jun 21 02:35:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 02:31:12 2022
Response via : Initial Calibration

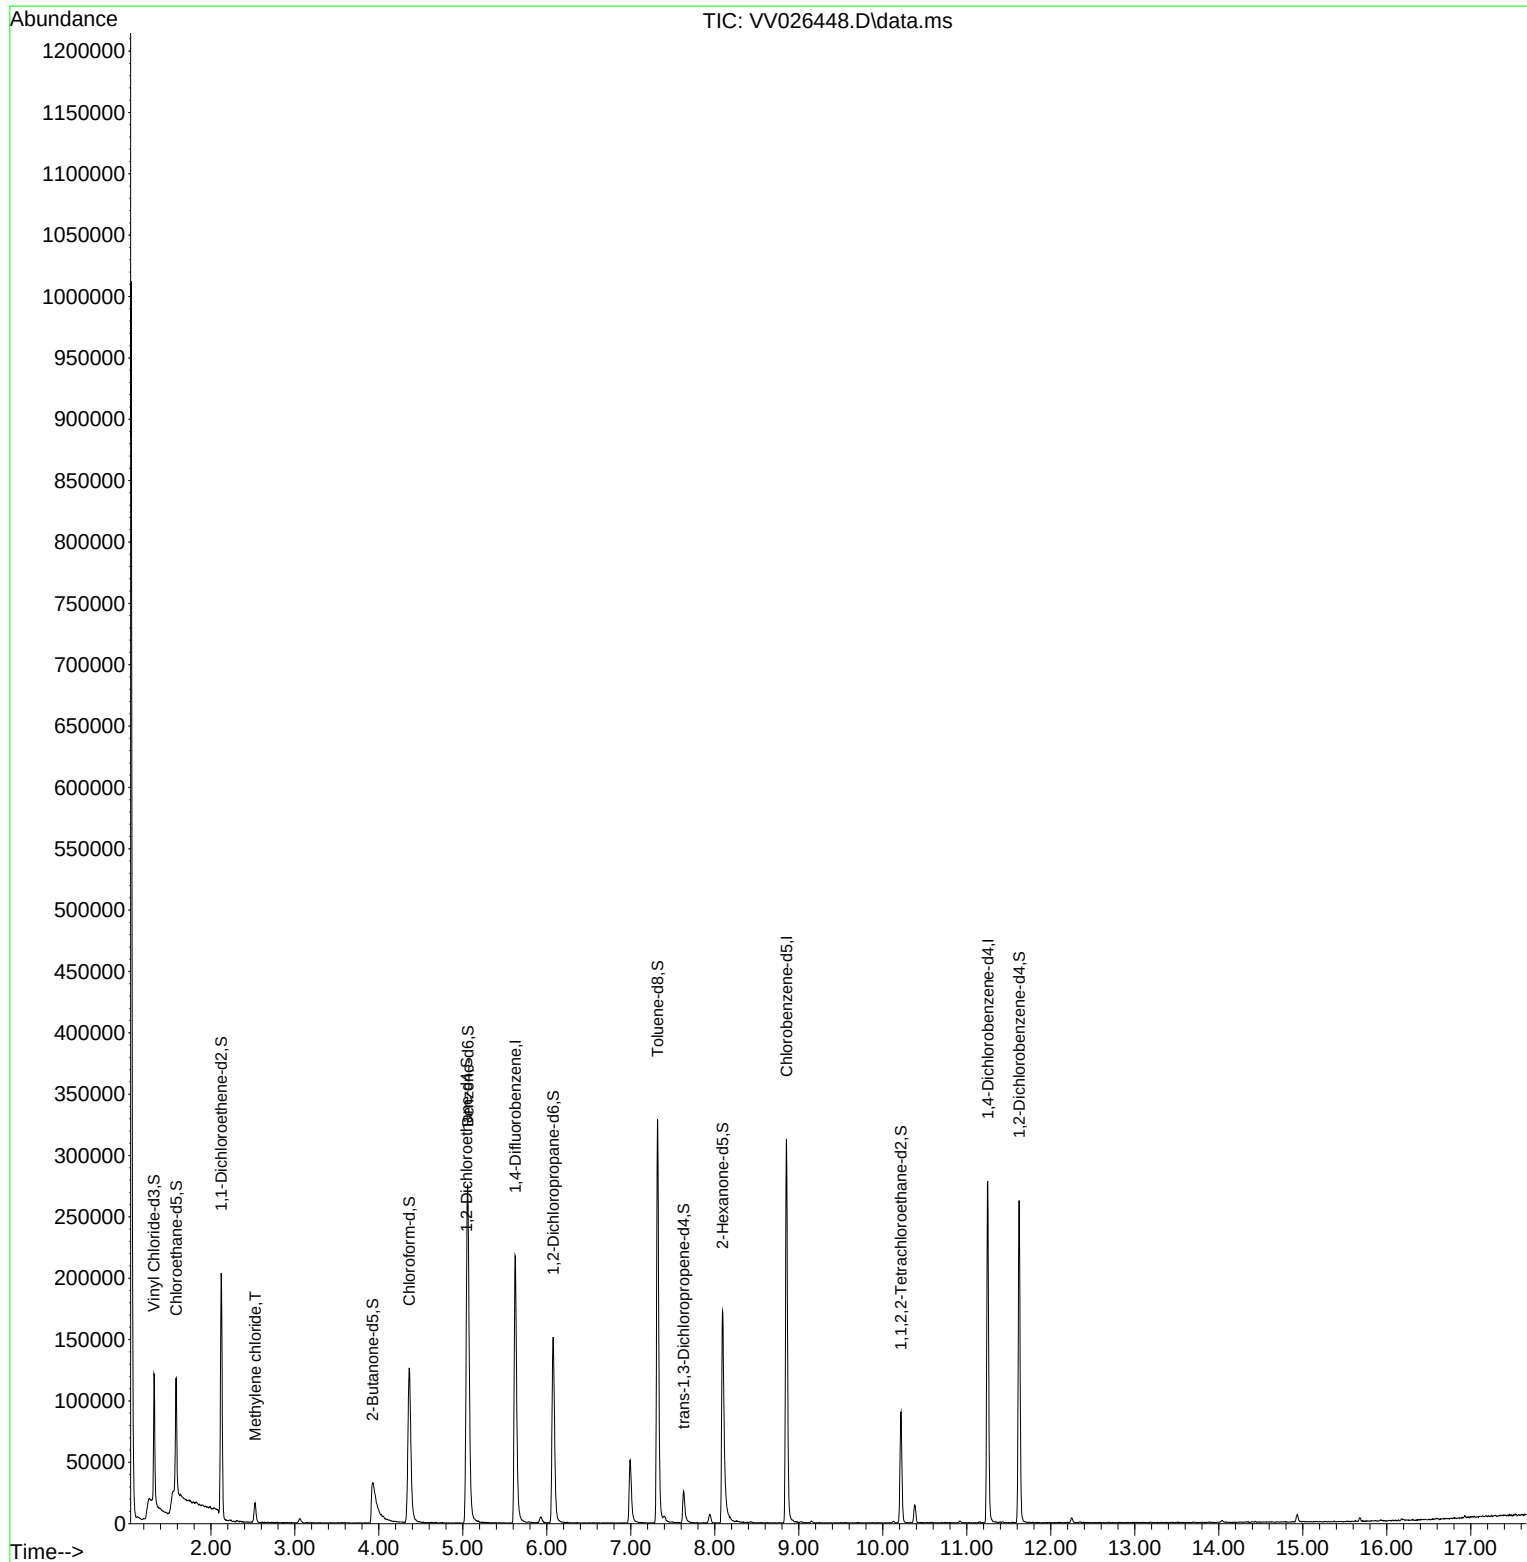

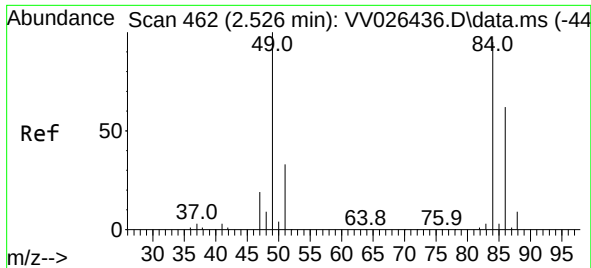

#16
Methylene chloride
Concen: 0.448 ug/L
RT: 2.526 min Scan# 462
Delta R.T. -0.000 min
Lab File: VV026448.D
Acq: 20 Jun 2022 16:12

Instrument :
MSVOA_V
ClientSampleId :
C0AK3

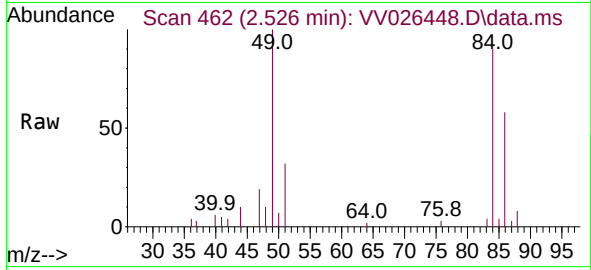

Tgt Ion: 84 Resp: 7019
Ion Ratio Lower Upper
84 100
86 65.0 44.0 81.8
49 111.4 77.3 143.7

