

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026449.D
 Acq On : 20 Jun 2022 16:34
 Operator : SY/MD
 Sample : N3256-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK4

Quant Time: Jun 21 02:35:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 02:31:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.629	114	188691	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	176147	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72418	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	67390	4.112	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.200%
7) Chloroethane-d5	1.587	69	59305	4.602	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.000%
11) 1,1-Dichloroethene-d2	2.127	63	100882	3.584	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.600%
20) 2-Butanone-d5	3.934	46	81756	51.123	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.240%
24) Chloroform-d	4.368	84	130541	5.434	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.600%
26) 1,2-Dichloroethane-d4	5.050	65	52251	5.141	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.800%
32) Benzene-d6	5.063	84	258007	5.479	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.600%
36) 1,2-Dichloropropane-d6	6.082	67	75504	5.493	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.800%
41) Toluene-d8	7.323	98	221111	5.149	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.000%
43) trans-1,3-Dichloroprop...	7.632	79	16090	3.610	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.200%
46) 2-Hexanone-d5	8.095	63	62171	46.179	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.360%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44594	5.267	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	65998	5.917	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.400%
Target Compounds						Qvalue
16) Methylene chloride	2.529	84	3553	0.234	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026449.D
Acq On : 20 Jun 2022 16:34
Operator : SY/MD
Sample : N3256-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK4

Quant Time: Jun 21 02:35:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 02:31:12 2022
Response via : Initial Calibration

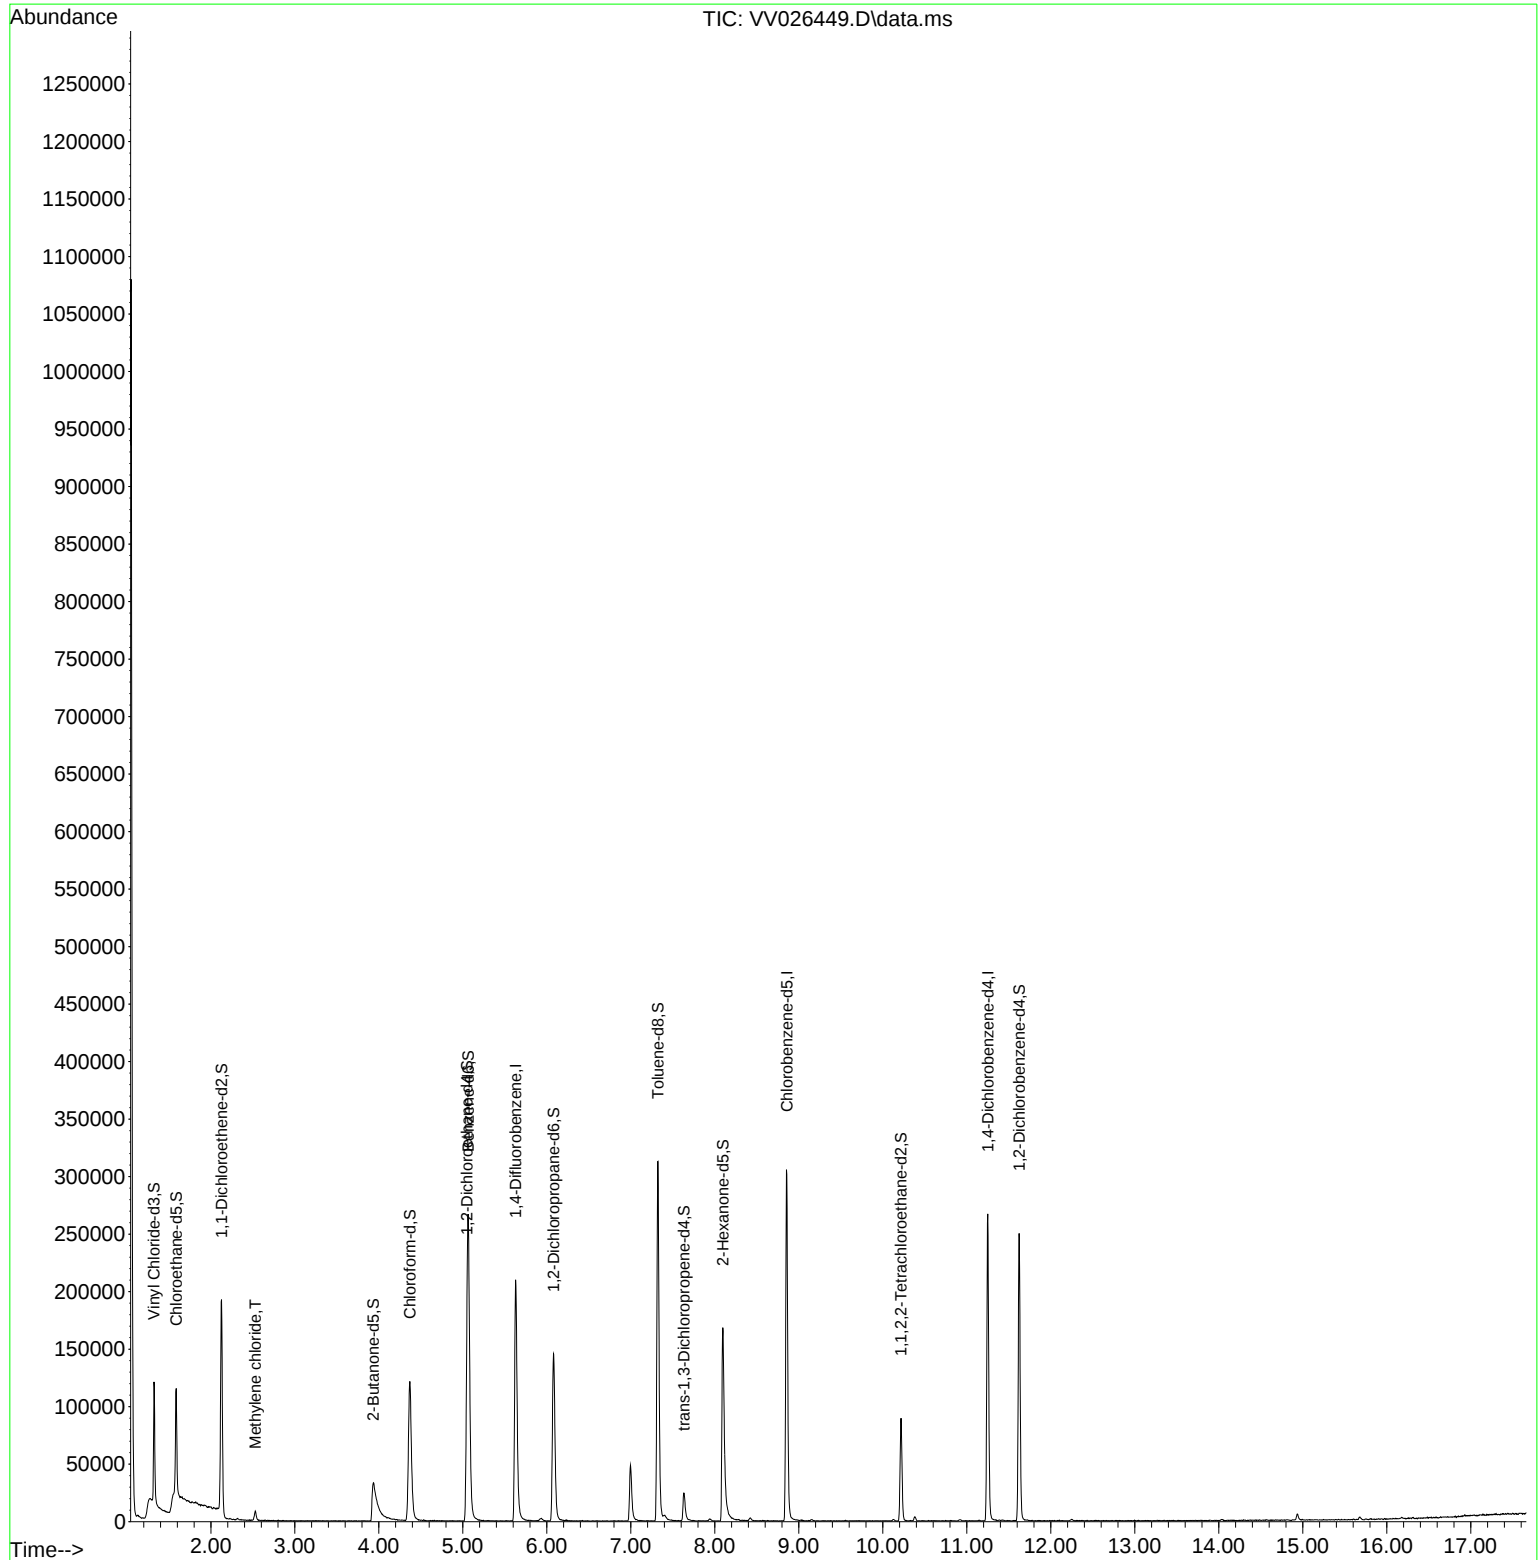

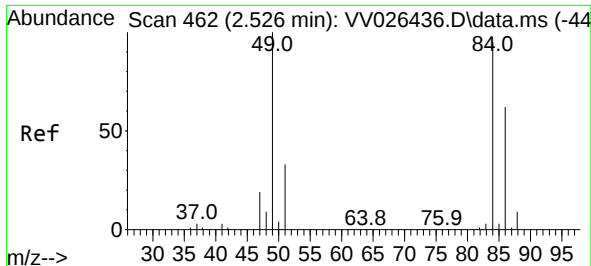

#16
Methylene chloride
Concen: 0.234 ug/L
RT: 2.529 min Scan# 463
Delta R.T. 0.003 min
Lab File: VV026449.D
Acq: 20 Jun 2022 16:34

Instrument :
MSVOA_V
ClientSampleId :
C0AK4

Tgt Ion: 84 Resp: 3553
Ion Ratio Lower Upper
84 100
86 67.9 44.0 81.8
49 98.3 77.3 143.7

