

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062022\
 Data File : VW026457.D
 Acq On : 20 Jun 2022 19:49
 Operator : SY/MD
 Sample : N3385-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3

Quant Time: Jun 21 05:39:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	194939	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	179410	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75024	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	76429	4.514	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.200%
7) Chloroethane-d5	1.584	69	64343	4.833	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.600%
11) 1,1-Dichloroethene-d2	2.124	63	107548	3.699	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.000%
20) 2-Butanone-d5	3.924	46	90971	55.062	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.120%
24) Chloroform-d	4.365	84	138859	5.595	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.000%
26) 1,2-Dichloroethane-d4	5.043	65	54929	5.232	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.600%
32) Benzene-d6	5.063	84	282094	5.881	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.600%
36) 1,2-Dichloropropane-d6	6.079	67	83325	5.952	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	119.000%
41) Toluene-d8	7.320	98	235932	5.394	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.800%
43) trans-1,3-Dichloroprop...	7.628	79	15477	3.410	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.200%
46) 2-Hexanone-d5	8.091	63	72523	52.889	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.780%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49601	5.752	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	72001	6.231	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	124.600%#
Target Compounds						
16) Methylene chloride	2.526	84	10247	0.652	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026457.D
Acq On : 20 Jun 2022 19:49
Operator : SY/MD
Sample : N3385-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3


Quant Time: Jun 21 05:39:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

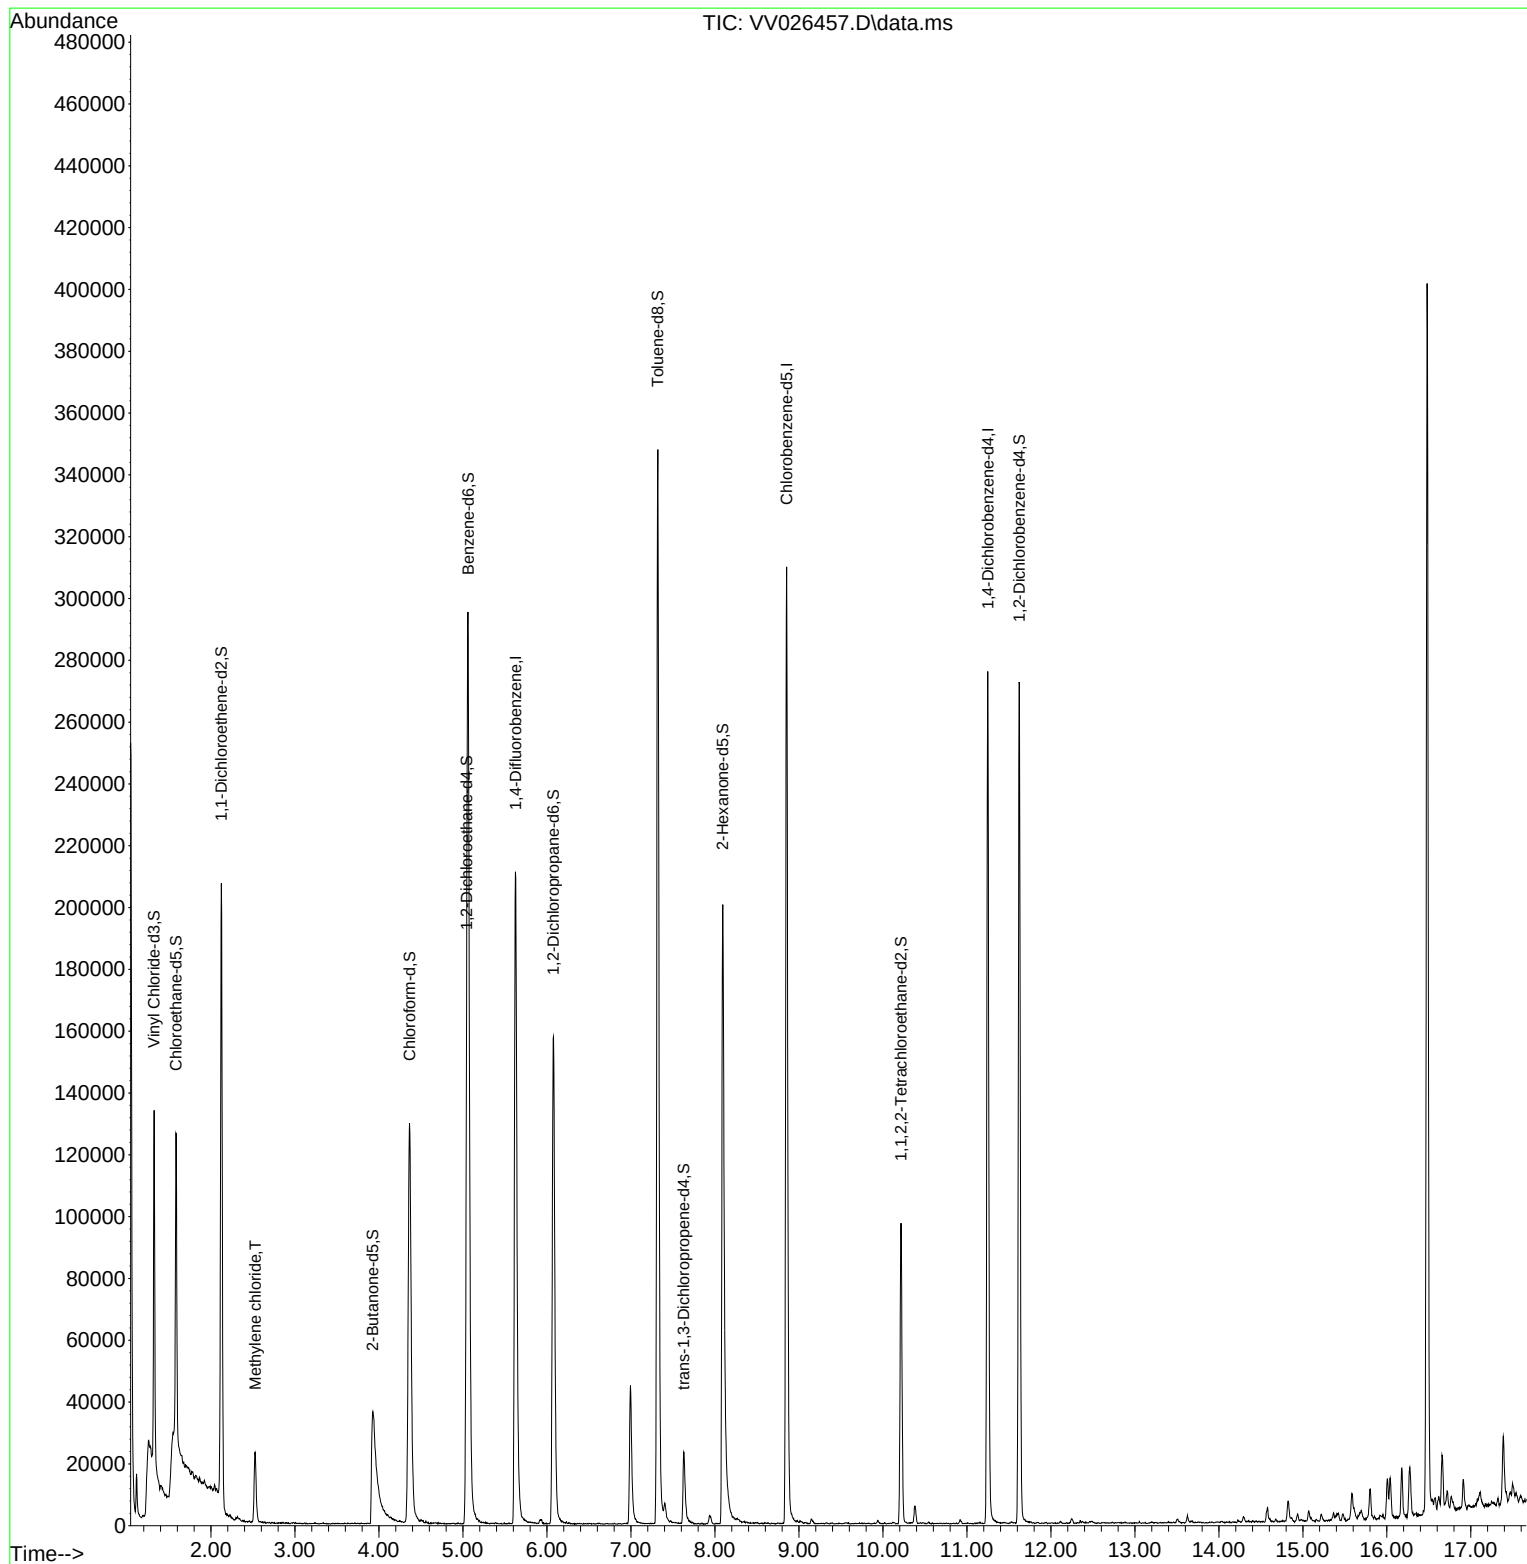

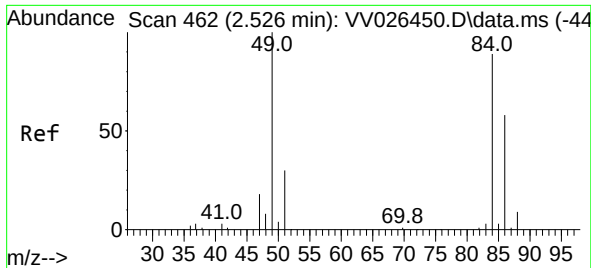

#16
Methylene chloride
Concen: 0.652 ug/L
RT: 2.526 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV026457.D
Acq: 20 Jun 2022 19:49

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

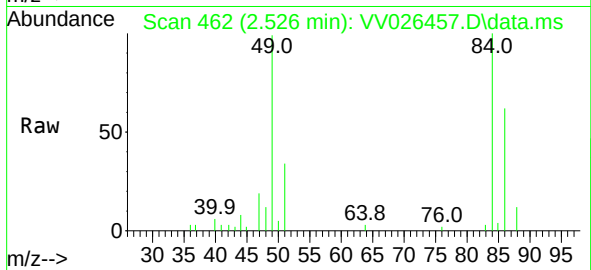

Tgt Ion: 84 Resp: 10247

Ion	Ratio	Lower	Upper
84	100		
86	61.7	44.0	81.8
49	98.7	77.3	143.7

