

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062022\
 Data File : VW026461.D
 Acq On : 20 Jun 2022 21:24
 Operator : SY/MD
 Sample : N3355-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D1

Quant Time: Jun 21 05:40:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.629	114	195479	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	175862	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73124	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	76497	4.505	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.200%
7) Chloroethane-d5	1.587	69	65565	4.911	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.200%
11) 1,1-Dichloroethene-d2	2.124	63	105548	3.620	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.400%
20) 2-Butanone-d5	3.928	46	99714	60.188	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.380%
24) Chloroform-d	4.365	84	142029	5.707	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.200%
26) 1,2-Dichloroethane-d4	5.047	65	58290	5.536	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.800%
32) Benzene-d6	5.063	84	284598	6.053	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	121.000%
36) 1,2-Dichloropropane-d6	6.075	67	84194	6.136	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	122.800%
41) Toluene-d8	7.320	98	232143	5.415	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.200%
43) trans-1,3-Dichloroprop...	7.632	79	15616	3.510	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.200%
46) 2-Hexanone-d5	8.095	63	77850	57.919	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	115.840%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	51765	6.124	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	122.400%#
66) 1,2-Dichlorobenzene-d4	11.622	152	72509	6.438	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	128.800%#
Target Compounds						Qvalue
3) Chloromethane	1.259	50	7182	0.443	ug/L	98
13) Acetone	2.214	43	11493	8.952	ug/L	90
63) 1,2,4-Trimethylbenzene	10.918	105	4875	0.159	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026461.D
Acq On : 20 Jun 2022 21:24
Operator : SY/MD
Sample : N3355-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D1

Quant Time: Jun 21 05:40:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration




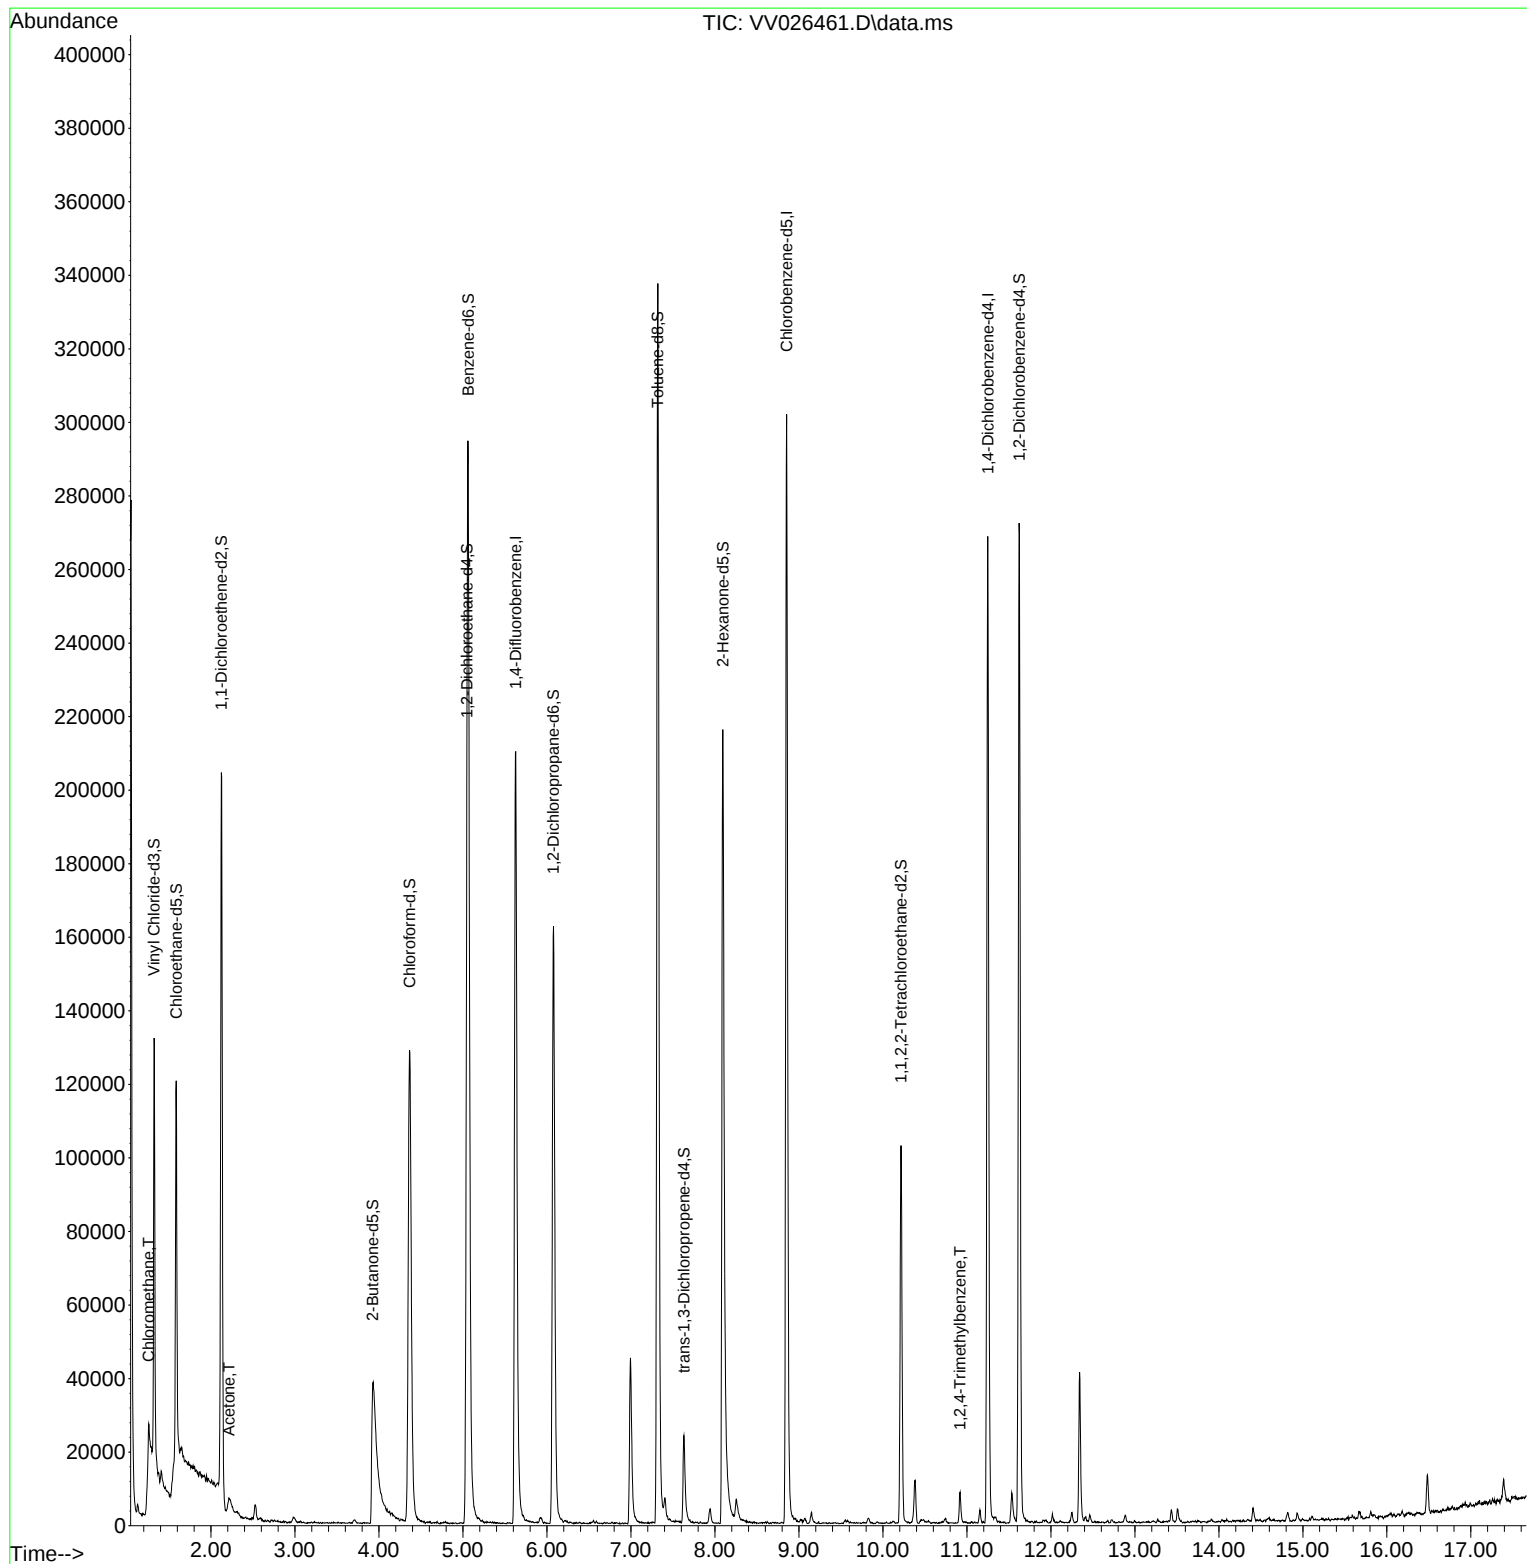


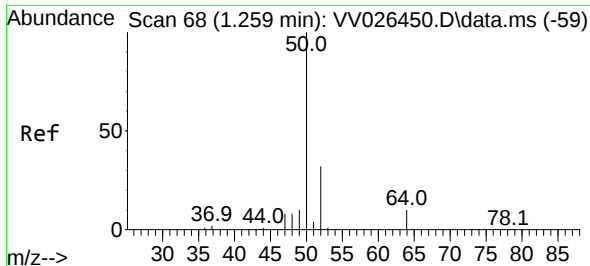

#3
Chloromethane
Concen: 0.443 ug/L
RT: 1.259 min Scan# 61
Delta R.T. -0.000 min
Lab File: VV026461.D
Acq: 20 Jun 2022 21:24




Instrument :
MSVOA_V
ClientSampleId :
EY0D1


Tgt Ion: 50 Resp: 7182
Ion Ratio Lower Upper
50 100
52 34.9 23.7 44.1

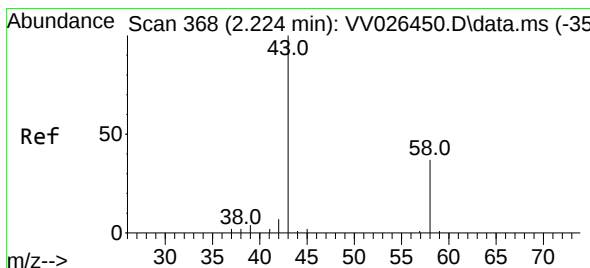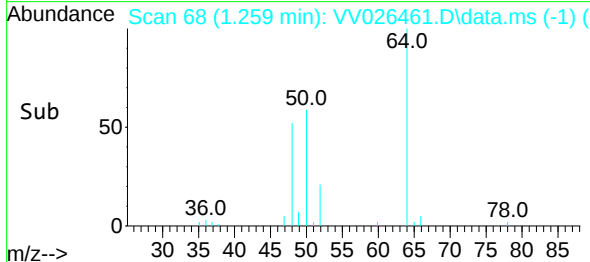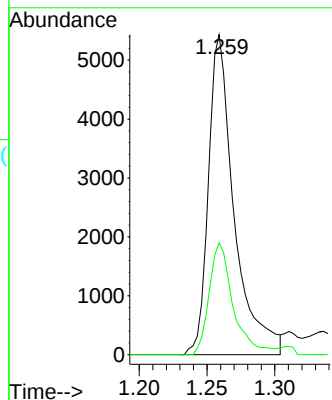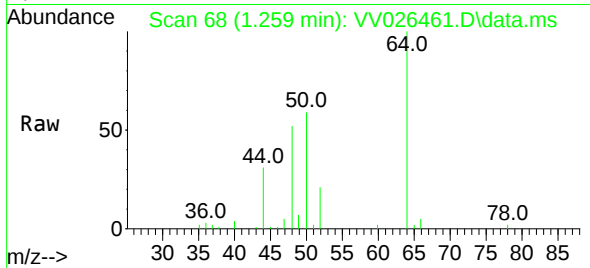

#13
Acetone
Concen: 8.952 ug/L
RT: 2.214 min Scan# 365
Delta R.T. -0.010 min
Lab File: VV026461.D
Acq: 20 Jun 2022 21:24

Tgt Ion: 43 Resp: 11493
Ion Ratio Lower Upper
43 100
58 24.3 0.0 60.0

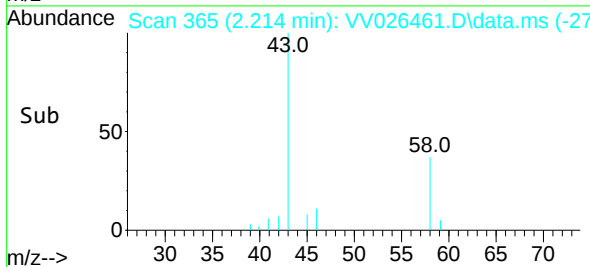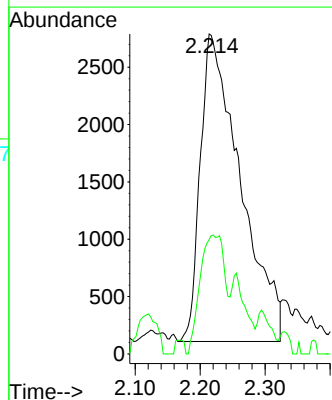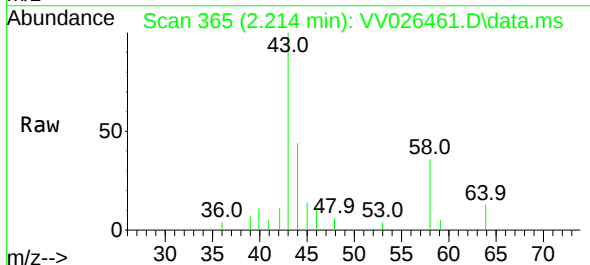

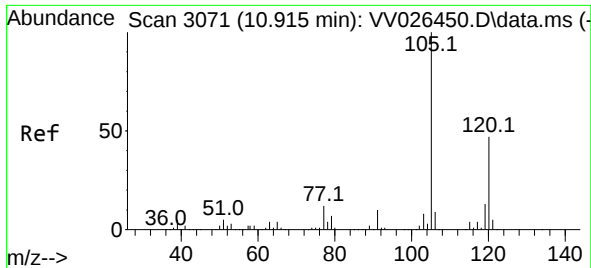

#63
 1,2,4-Trimethylbenzene
 Concen: 0.159 ug/L
 RT: 10.918 min Scan# 3072
 Delta R.T. 0.003 min
 Lab File: VV026461.D
 Acq: 20 Jun 2022 21:24

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D1

Tgt Ion:105 Resp: 4875
 Ion Ratio Lower Upper
 105 100
 120 46.6 36.9 55.3

