

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062022\
 Data File : VW026465.D
 Acq On : 20 Jun 2022 23:00
 Operator : SY/MD
 Sample : N3401-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE0

Quant Time: Jun 21 05:41:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	143175	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	135191	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55312	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	69666	5.602	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	112.000%	
7) Chloroethane-d5	1.584	69	61049	6.243	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	124.800%	
11) 1,1-Dichloroethene-d2	2.124	63	103629	4.853	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	97.000%	
20) 2-Butanone-d5	3.925	46	94859	78.174	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	156.340%#	
24) Chloroform-d	4.365	84	131502	7.215	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	144.200%#	
26) 1,2-Dichloroethane-d4	5.047	65	55694	7.222	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	144.400%#	
32) Benzene-d6	5.060	84	266616	7.377	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	147.600%#	
36) 1,2-Dichloropropane-d6	6.076	67	79552	7.541	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	150.800%#	
41) Toluene-d8	7.320	98	221795	6.730	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	134.600%#	
43) trans-1,3-Dichloroprop...	7.629	79	15100	4.414	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.200%	
46) 2-Hexanone-d5	8.092	63	69192	66.964	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	133.920%#	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47962	7.381	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	147.600%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	69035	8.103	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	162.000%#	
Target Compounds						
42) Toluene	7.400	91	8242	0.226	ug/L	95
53) m,p-Xylene	9.153	106	1413	0.099	ug/L	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026465.D
Acq On : 20 Jun 2022 23:00
Operator : SY/MD
Sample : N3401-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Time: Jun 21 05:41:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

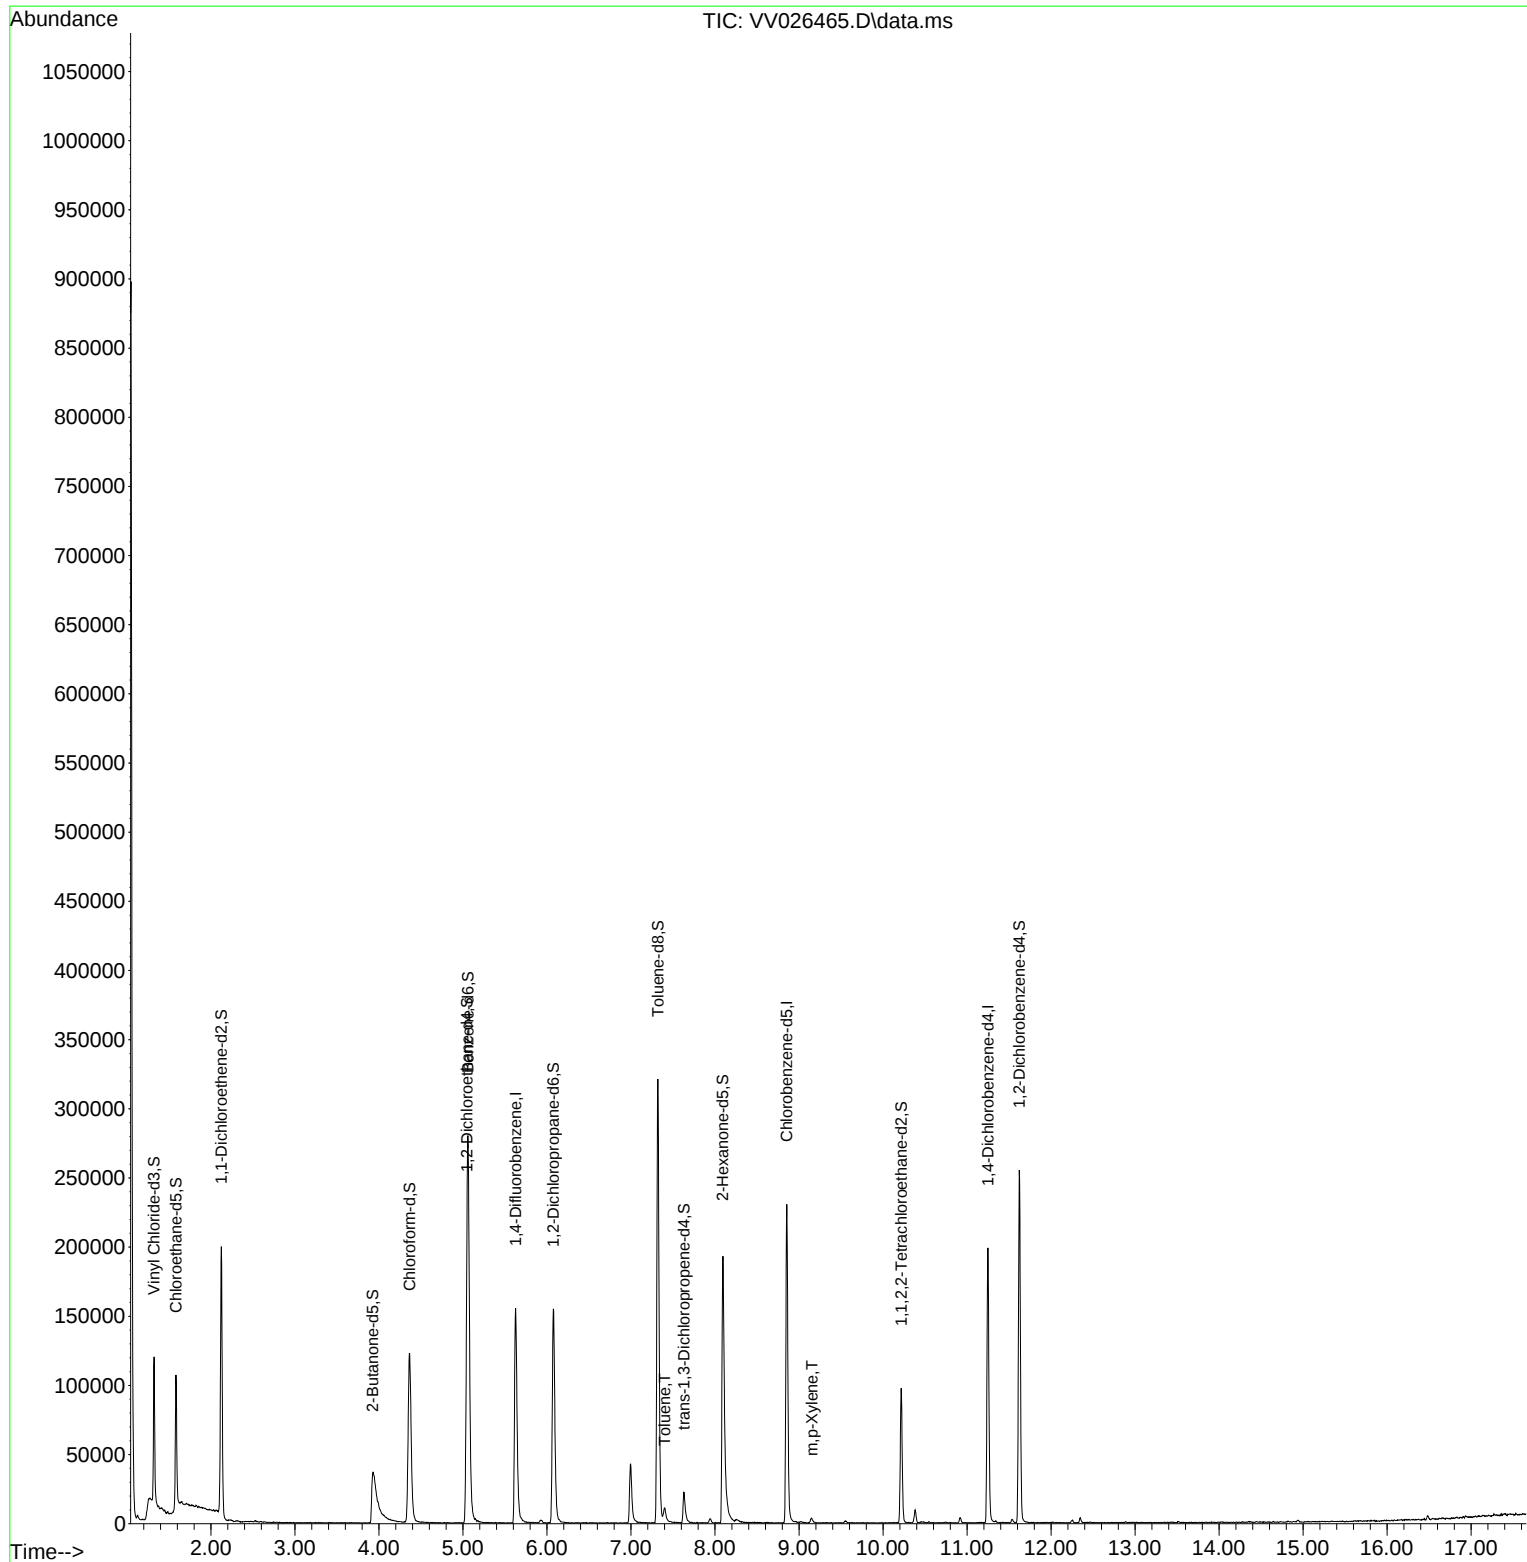

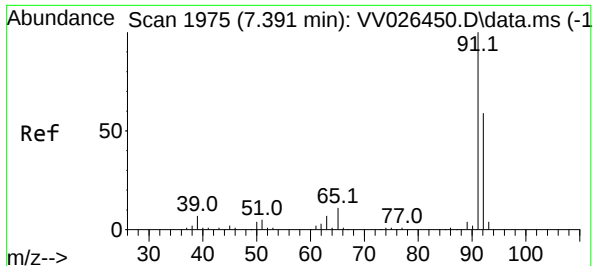

#42

Toluene

Concen: 0.226 ug/L

RT: 7.400 min Scan# 1975

Delta R.T. 0.010 min

Lab File: VV026465.D

Acq: 20 Jun 2022 23:00

Instrument :

MSVOA_V

ClientSampleId :





C0AE0

Tgt Ion: 91 Resp: 8242

Ion Ratio Lower Upper

91 100

92 61.3 40.1 74.5

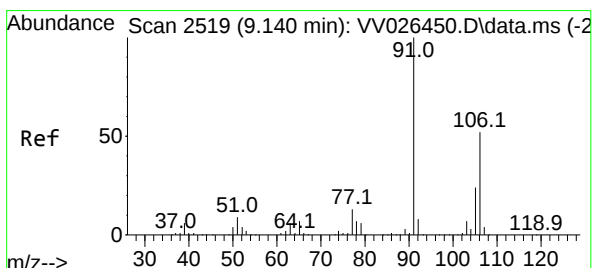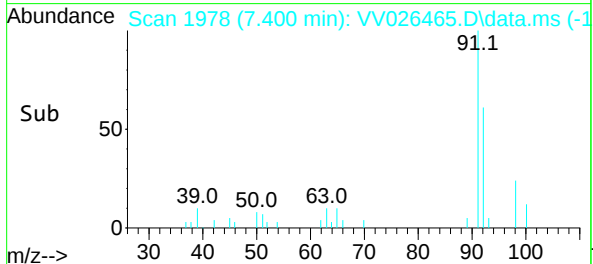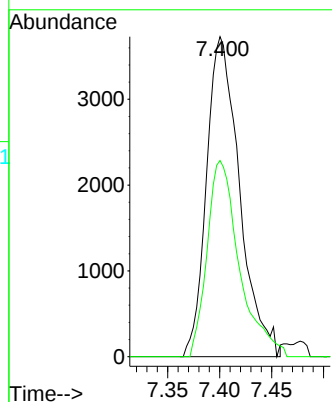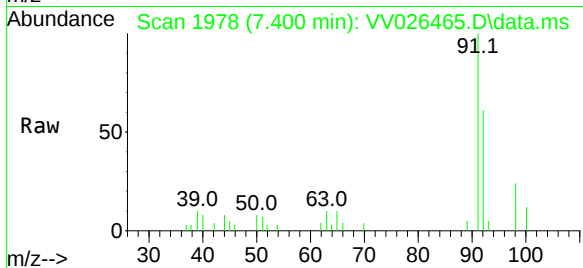

#53

m,p-Xylene

Concen: 0.099 ug/L

RT: 9.153 min Scan# 2523

Delta R.T. 0.013 min

Lab File: VV026465.D

Acq: 20 Jun 2022 23:00

Tgt Ion: 106 Resp: 1413

Ion Ratio Lower Upper

106 100

91 147.9 141.3 262.3

