

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026468.D
 Acq On : 21 Jun 2022 00:12
 Operator : SY/MD
 Sample : N3401-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD7

Quant Time: Jun 21 05:42:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 21 05:26:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	184493	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	174423	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	70850	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	63746	3.978	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.600%
7) Chloroethane-d5	1.584	69	56385	4.475	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.600%
11) 1,1-Dichloroethene-d2	2.124	63	92892	3.376	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.600%
20) 2-Butanone-d5	3.931	46	88788	56.784	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.560%
24) Chloroform-d	4.362	84	127652	5.435	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.600%
26) 1,2-Dichloroethane-d4	5.043	65	50927	5.125	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
32) Benzene-d6	5.060	84	244153	5.236	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%
36) 1,2-Dichloropropane-d6	6.076	67	73193	5.378	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.600%
41) Toluene-d8	7.320	98	202546	4.763	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%
43) trans-1,3-Dichloroprop...	7.629	79	16545	3.749	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.000%
46) 2-Hexanone-d5	8.095	63	68006	51.013	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.020%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45949	5.481	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	64329	5.895	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.800%
Target Compounds						
25) Chloroform	4.391	83	40369	1.726	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026468.D
Acq On : 21 Jun 2022 00:12
Operator : SY/MD
Sample : N3401-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD7

Quant Time: Jun 21 05:42:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 21 05:26:17 2022
Response via : Initial Calibration

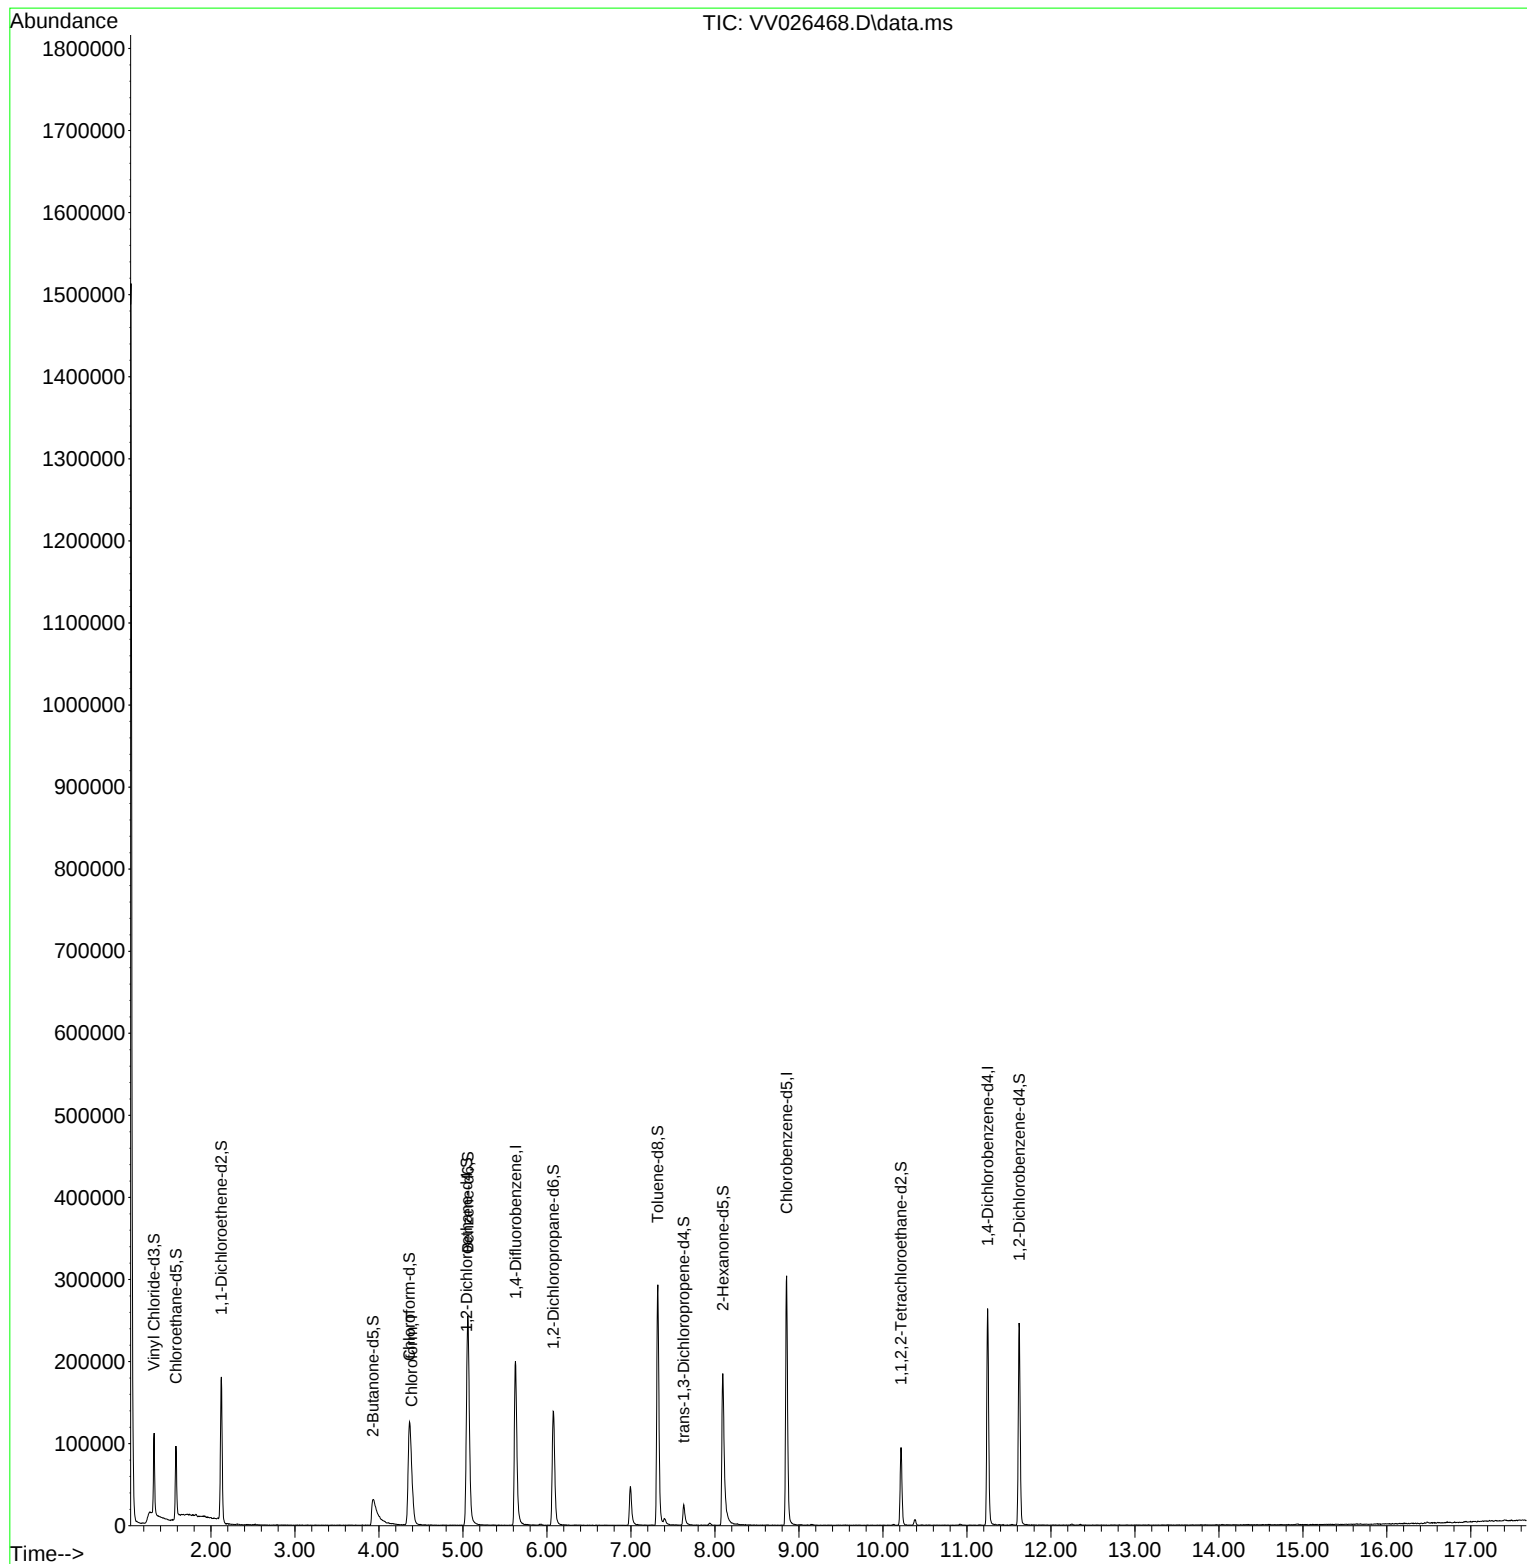

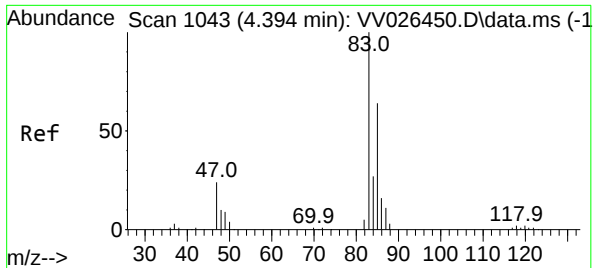

#25
Chloroform
Concen: 1.726 ug/L
RT: 4.391 min Scan# 10
Delta R.T. -0.003 min
Lab File: VV026468.D
Acq: 21 Jun 2022 00:12

Instrument :
MSVOA_V
ClientSampleId :
C0AD7

Tgt Ion: 83 Resp: 40369
Ion Ratio Lower Upper
83 100
85 67.4 46.5 86.3

