

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026437.D
 Acq On : 20 Jun 2022 11:41
 Operator : SY/MD
 Sample : VV0620WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK380

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.326	82	89	105	rVB	132470	142245	17.99%	2.359%
2	1.587	163	170	181	rBV	104836	119435	15.11%	1.981%
3	2.127	328	338	357	rVB	222418	328477	41.55%	5.448%
4	2.526	451	462	482	rVB2	18484	32857	4.16%	0.545%
5	3.931	884	899	929	rBV2	36334	154377	19.53%	2.560%
6	4.362	1016	1033	1057	rBV	139767	347906	44.01%	5.770%
7	5.056	1233	1249	1276	rBV3	321848	790569	100.00%	13.112%
8	5.622	1414	1425	1452	rBV	261735	539264	68.21%	8.944%
9	6.075	1552	1566	1602	rBV2	172074	360966	45.66%	5.987%
10	6.992	1839	1851	1873	rBV	65783	125746	15.91%	2.086%
11	7.317	1940	1952	1971	rBV	394735	696205	88.06%	11.547%
12	7.628	2039	2049	2076	rBV	34025	62691	7.93%	1.040%
13	8.091	2183	2193	2233	rBV	206870	434779	55.00%	7.211%
14	8.853	2419	2430	2454	rBV	368594	613214	77.57%	10.171%
15	10.217	2843	2854	2867	rBV	105127	167744	21.22%	2.782%
16	11.246	3164	3174	3195	rBV	338687	526992	66.66%	8.741%
17	11.622	3279	3291	3307	rBV	315680	498236	63.02%	8.264%
18	14.934	4306	4321	4339	rBV	33660	58926	7.45%	0.977%
19	15.680	4544	4553	4563	rBV	18542	28599	3.62%	0.474%


Sum of corrected areas: 6029228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026437.D
Acq On : 20 Jun 2022 11:41
Operator : SY/MD
Sample : VV0620WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

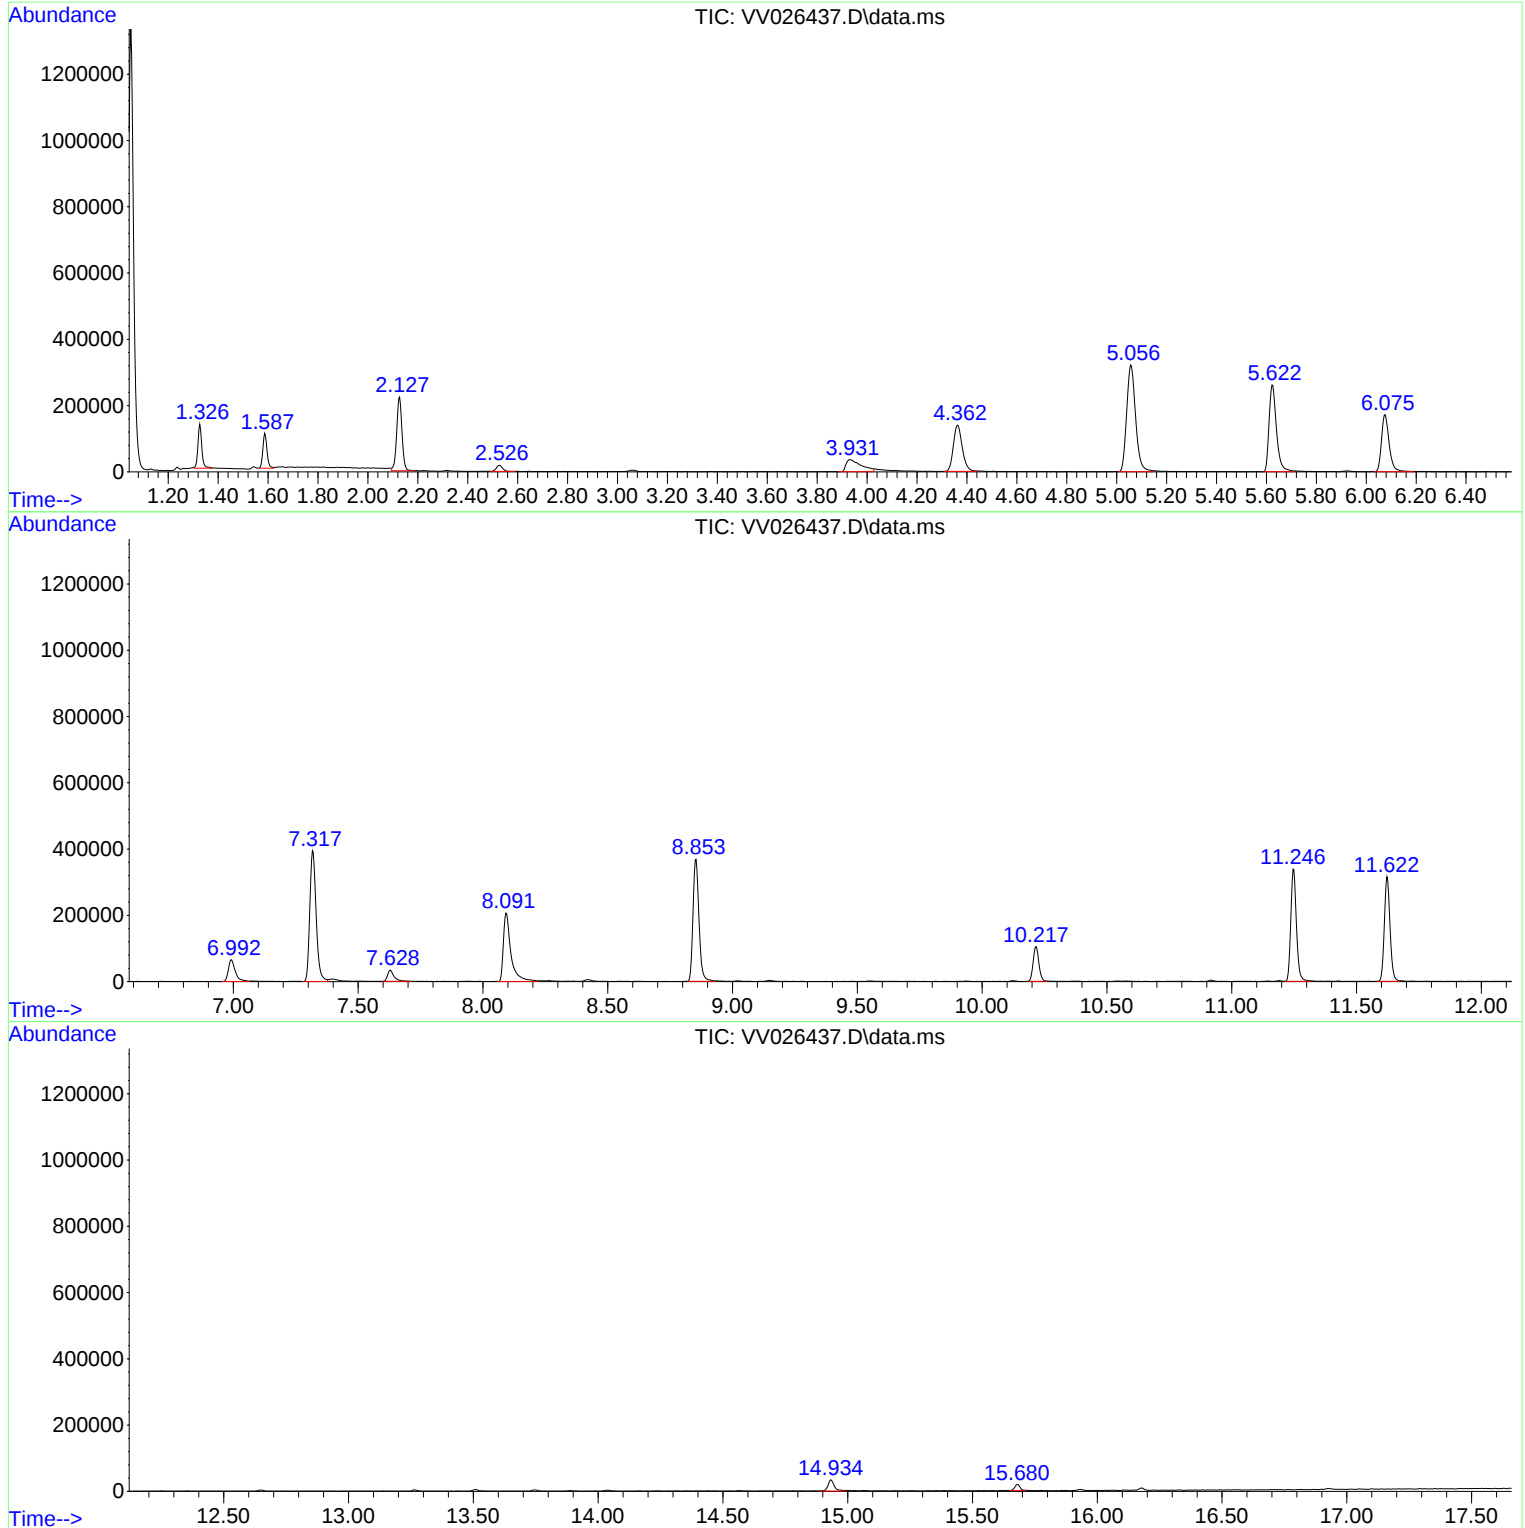

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV062437.D
Acq On : 20 Jun 2022 11:41
Operator : SY/MD
Sample : VV0620WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Phenol, p-tert-butyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.934	0.56 ug/L	58926	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, p-tert-butyl-	150	C10H14O	000098-54-4	96
2			Phenol, p-tert-butyl-	150	C10H14O	000098-54-4	96
3			Phenol, m-tert-butyl-	150	C10H14O	000585-34-2	94
4			Phenol, m-tert-butyl-	150	C10H14O	000585-34-2	91
5			Phenol, p-tert-butyl-	150	C10H14O	000098-54-4	90

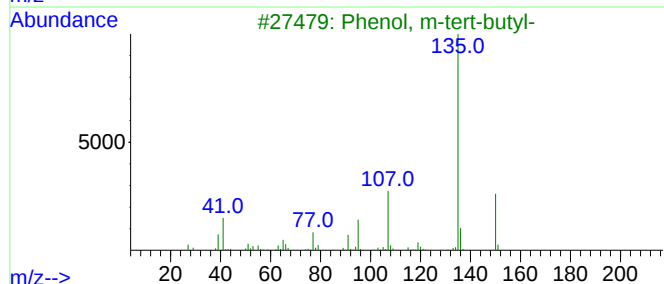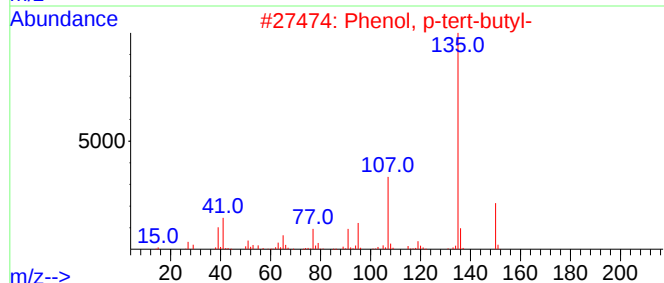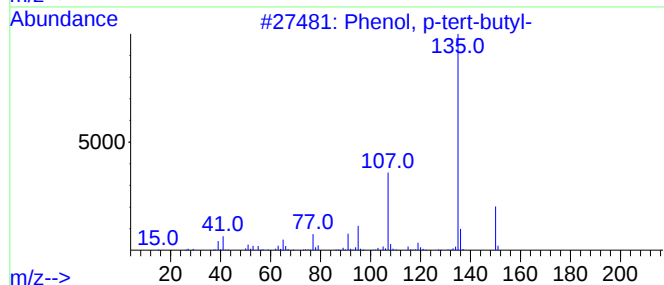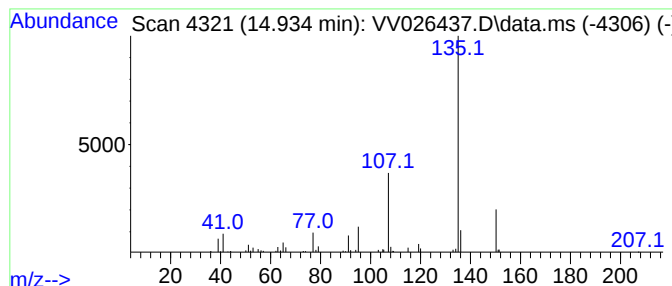

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026437.D
Acq On : 20 Jun 2022 11:41
Operator : SY/MD
Sample : VV0620WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, p-tert-...	14.934	0.6	ug/L	58926	3	11.249	526992	5.0