

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026448.D
 Acq On : 20 Jun 2022 16:12
 Operator : SY/MD
 Sample : N3256-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.265	56	70	74	rBV2	16276	37513	5.55%	0.728%
2	1.323	82	88	101	rVB	108435	121092	17.91%	2.351%
3	1.545	145	157	158	rBV6	16804	23557	3.48%	0.457%
4	1.587	163	170	183	rVB	98394	131139	19.39%	2.546%
5	2.124	328	337	352	rVB	201075	285786	42.26%	5.549%
6	2.526	452	462	477	rVB2	16033	27414	4.05%	0.532%
7	3.928	886	898	927	rBV2	32771	134039	19.82%	2.603%
8	4.362	1017	1033	1065	rBV	126015	315836	46.70%	6.132%
9	5.056	1233	1249	1286	rBV2	275692	676287	100.00%	13.131%
10	5.622	1413	1425	1450	rBV	217776	440875	65.19%	8.560%
11	5.928	1511	1520	1535	rVB8	4851	10896	1.61%	0.212%
12	6.075	1552	1566	1597	rBV	151502	316897	46.86%	6.153%
13	6.992	1840	1851	1875	rBV2	51236	100027	14.79%	1.942%
14	7.317	1939	1952	1971	rBV	328963	571507	84.51%	11.096%
15	7.628	2039	2049	2074	rBV2	26051	49809	7.37%	0.967%
16	7.940	2136	2146	2159	rVB2	7020	13005	1.92%	0.253%
17	8.091	2183	2193	2220	rBV	172893	354174	52.37%	6.877%
18	8.853	2418	2430	2451	rBV	312916	517809	76.57%	10.054%
19	10.217	2841	2854	2874	rBV	90374	142359	21.05%	2.764%
20	10.381	2893	2905	2916	rBV3	14695	24748	3.66%	0.481%
21	11.249	3163	3175	3195	rBV	278235	434177	64.20%	8.430%
22	11.622	3279	3291	3310	rBV	262476	411448	60.84%	7.989%
23	14.934	4313	4321	4331	rBV3	6132	9962	1.47%	0.193%




Sum of corrected areas: 5150356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026448.D
Acq On : 20 Jun 2022 16:12
Operator : SY/MD
Sample : N3256-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

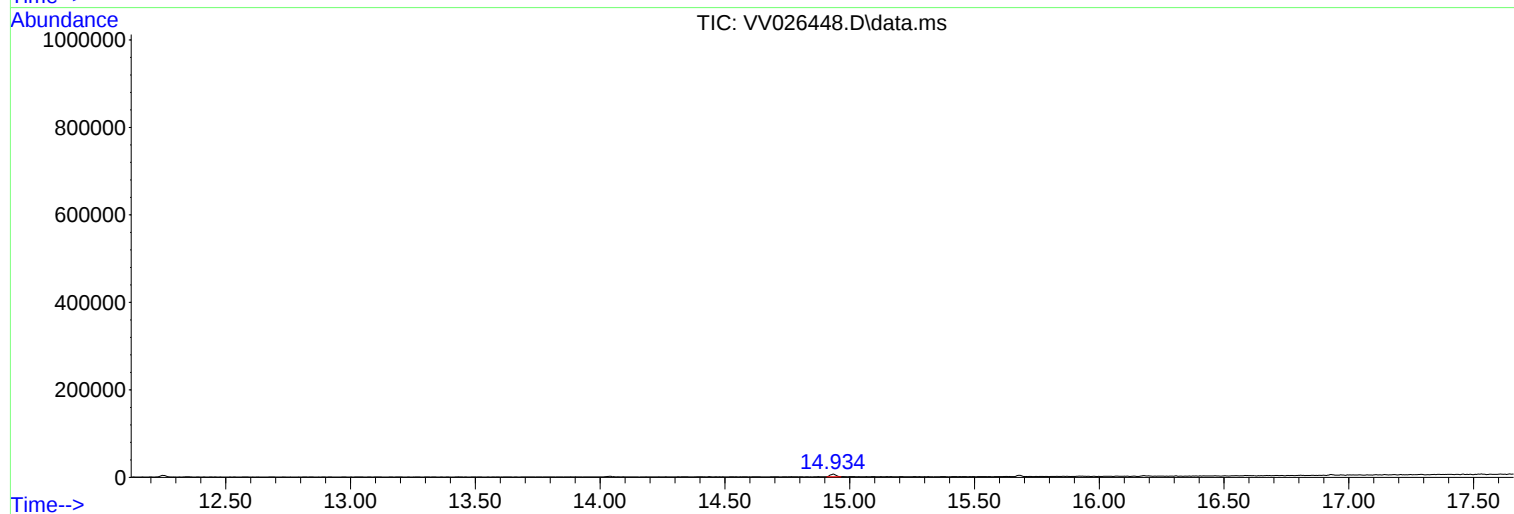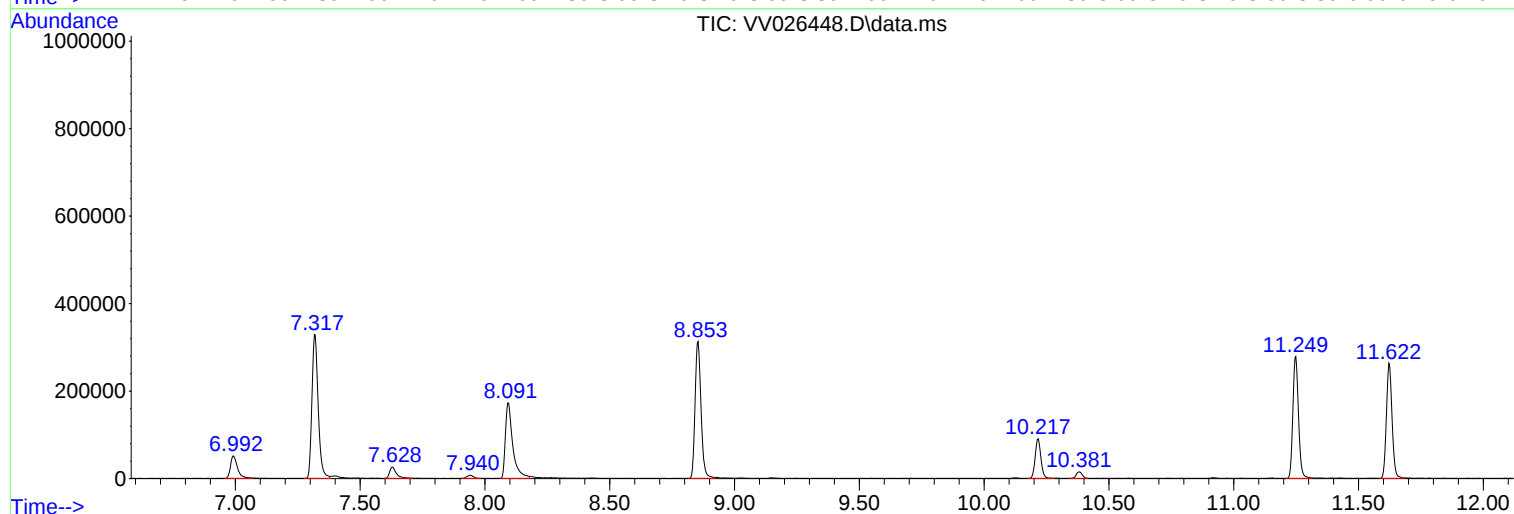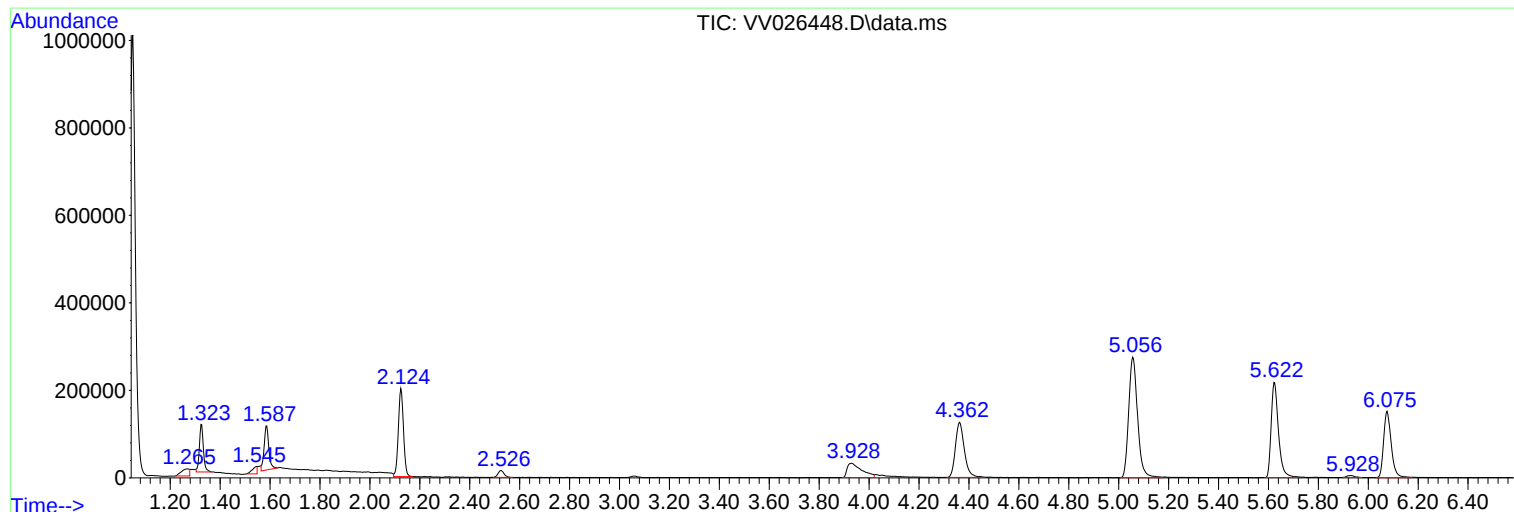

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026448.D
Acq On : 20 Jun 2022 16:12
Operator : SY/MD
Sample : N3256-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026448.D
Acq On : 20 Jun 2022 16:12
Operator : SY/MD
Sample : N3256-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc