

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026451.D
 Acq On : 20 Jun 2022 17:25
 Operator : SY/MD
 Sample : VV0620WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK381

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.269	54	71	74	rBV2	17668	39454	6.40%	0.802%
2	1.326	82	89	111	rVB	95901	116497	18.90%	2.369%
3	1.587	147	170	184	rBV2	105893	208051	33.76%	4.230%
4	2.124	328	337	355	rVB	175393	262383	42.57%	5.335%
5	2.526	454	462	474	rVB3	5772	10502	1.70%	0.214%
6	3.928	885	898	936	rBV2	37611	159640	25.90%	3.246%
7	4.365	1017	1034	1061	rBV	109915	280591	45.53%	5.705%
8	5.059	1234	1250	1279	rBV2	249559	616341	100.00%	12.531%
9	5.625	1413	1426	1459	rBV	203762	420732	68.26%	8.554%
10	6.075	1554	1566	1595	rBV	140662	290640	47.16%	5.909%
11	6.992	1841	1851	1873	rBV2	46192	90184	14.63%	1.834%
12	7.320	1940	1953	1972	rBV	286407	510592	82.84%	10.381%
13	7.628	2040	2049	2071	rBV	23755	45081	7.31%	0.917%
14	8.091	2184	2193	2230	rBV	185278	386452	62.70%	7.857%
15	8.419	2286	2295	2310	rVB2	5446	9639	1.56%	0.196%
16	8.853	2415	2430	2457	rBV	300507	499683	81.07%	10.159%
17	10.214	2839	2853	2871	rBV	93684	147794	23.98%	3.005%
18	11.249	3164	3175	3201	rBV	271695	431572	70.02%	8.775%
19	11.622	3278	3291	3316	rBV	248400	392636	63.70%	7.983%




Sum of corrected areas: 4918464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026451.D
Acq On : 20 Jun 2022 17:25
Operator : SY/MD
Sample : VV0620WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

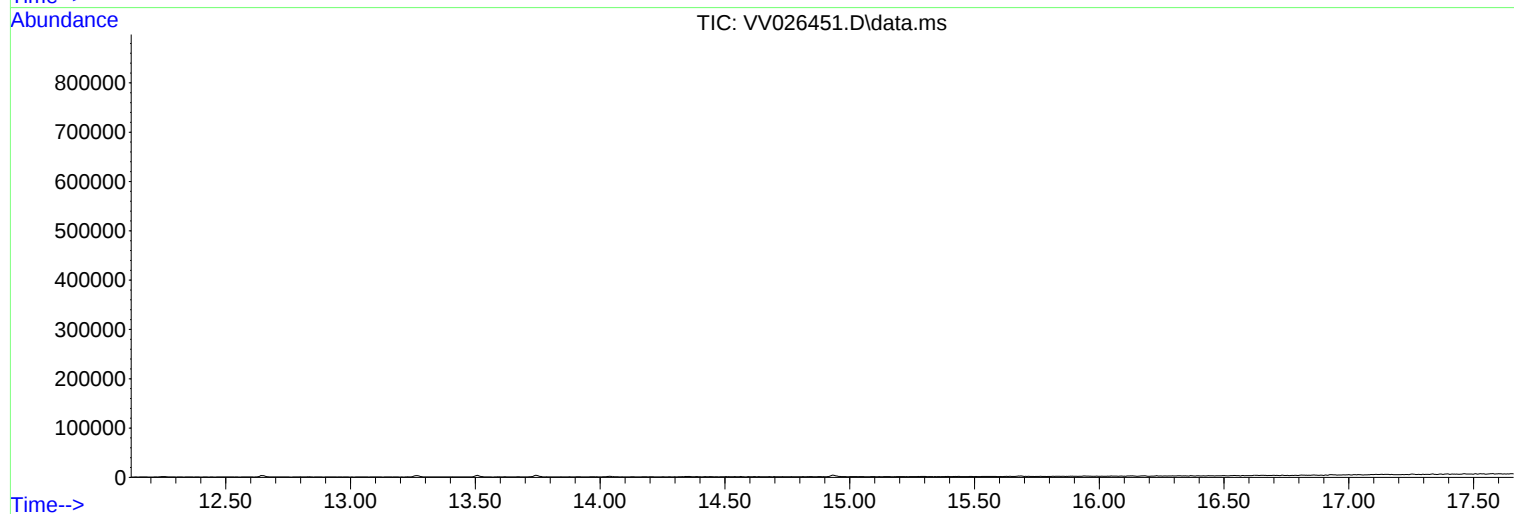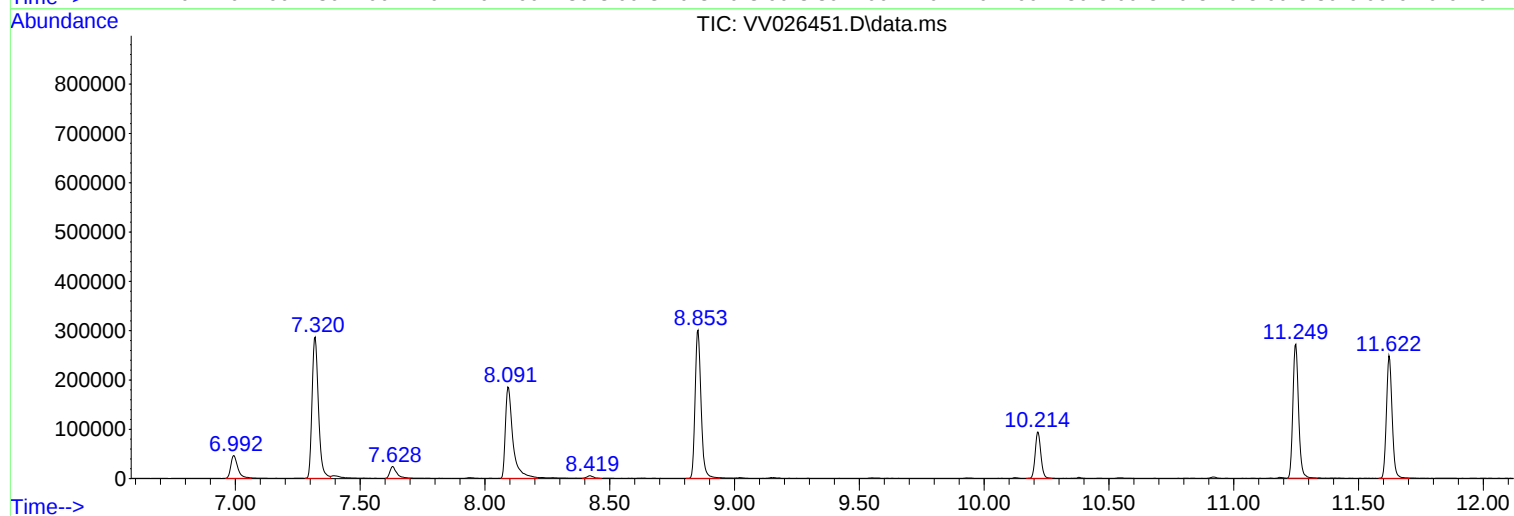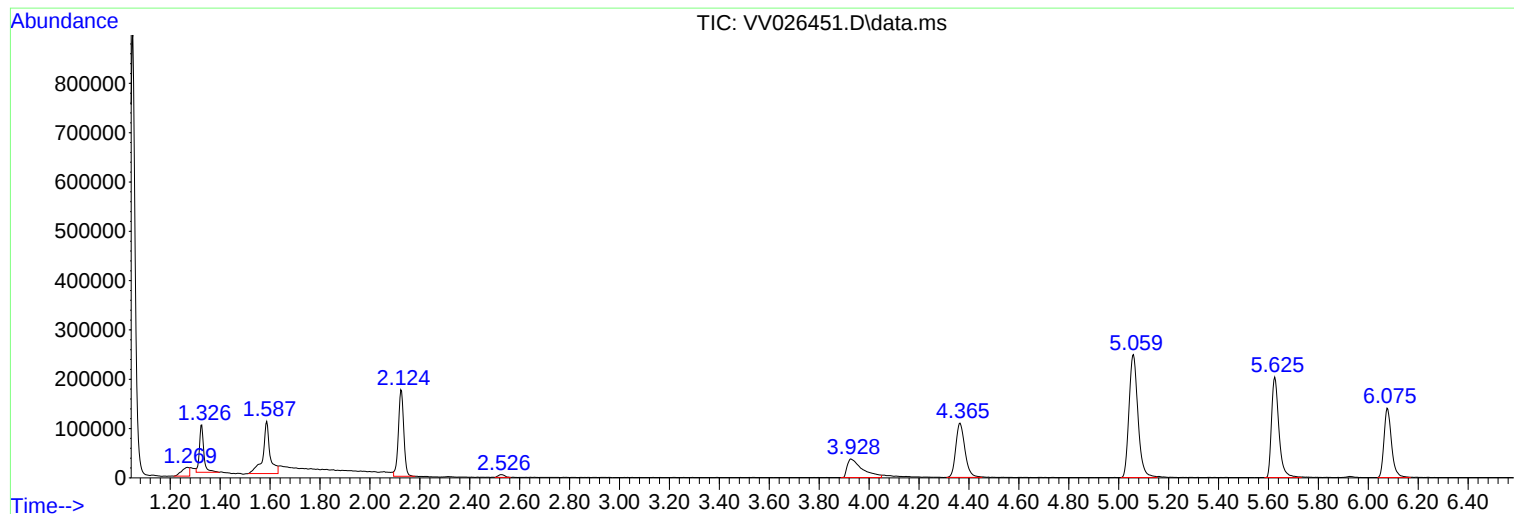

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026451.D
Acq On : 20 Jun 2022 17:25
Operator : SY/MD
Sample : VV0620WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026451.D
Acq On : 20 Jun 2022 17:25
Operator : SY/MD
Sample : VV0620WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------