

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026458.D
 Acq On : 20 Jun 2022 20:13
 Operator : SY/MD
 Sample : N3318-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	55	74	81	rBV2	16211	56889	8.44%	1.071%
2	1.323	82	88	106	rVB	108333	129138	19.15%	2.431%
3	1.584	151	169	179	rBV	103530	161034	23.88%	3.032%
4	2.124	328	337	358	rVB	189784	283822	42.09%	5.344%
5	3.931	888	899	935	rBV	37223	160971	23.87%	3.031%
6	4.365	1017	1034	1060	rBV	118185	301759	44.75%	5.681%
7	5.060	1231	1250	1285	rBV2	274806	674389	100.00%	12.697%
8	5.626	1415	1426	1454	rBV	210762	436919	64.79%	8.226%
9	6.079	1554	1567	1597	rBV	149369	314723	46.67%	5.925%
10	6.995	1839	1852	1870	rBV	50090	95910	14.22%	1.806%
11	7.320	1941	1953	1971	rBV	321564	559134	82.91%	10.527%
12	7.629	2039	2049	2065	rBV2	25897	47951	7.11%	0.903%
13	8.095	2184	2194	2221	rBV	193347	392099	58.14%	7.382%
14	8.854	2416	2430	2458	rBV	309110	512317	75.97%	9.645%
15	10.217	2843	2854	2879	rBV	96163	151568	22.47%	2.854%
16	11.249	3164	3175	3194	rBV	282043	432225	64.09%	8.138%
17	11.622	3280	3291	3313	rBV	260243	407333	60.40%	7.669%
18	16.480	4789	4802	4816	rBV	106407	170113	25.22%	3.203%
19	17.387	5076	5084	5094	rBV3	14014	23215	3.44%	0.437%




Sum of corrected areas: 5311509

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026458.D
Acq On : 20 Jun 2022 20:13
Operator : SY/MD
Sample : N3318-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

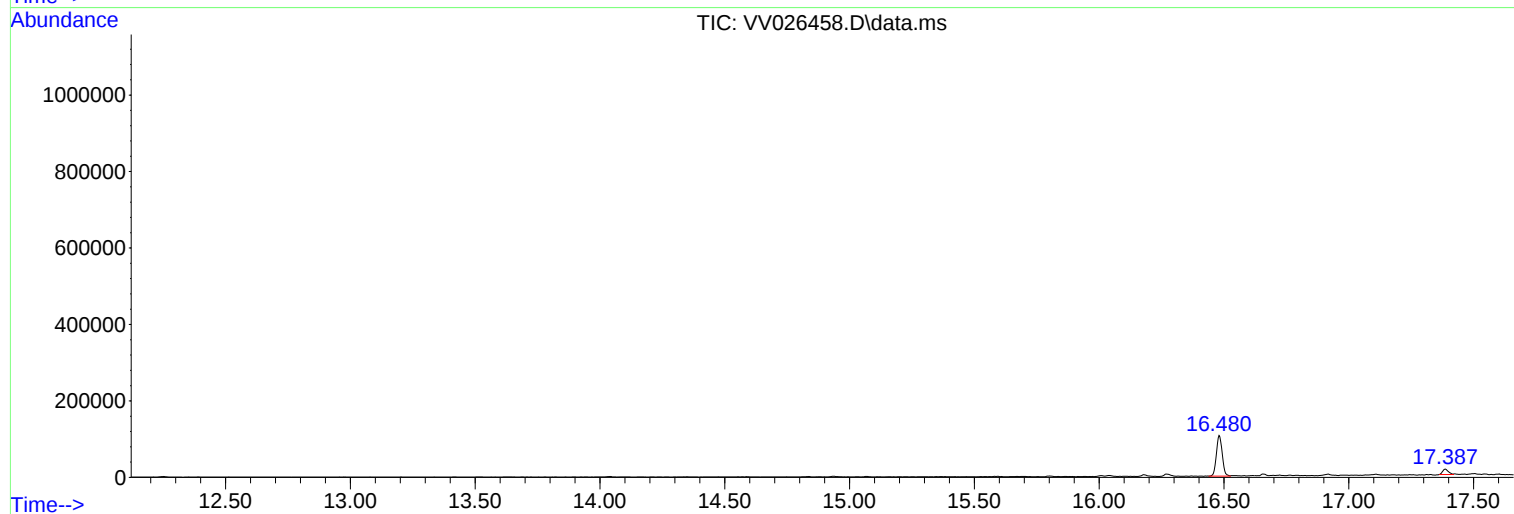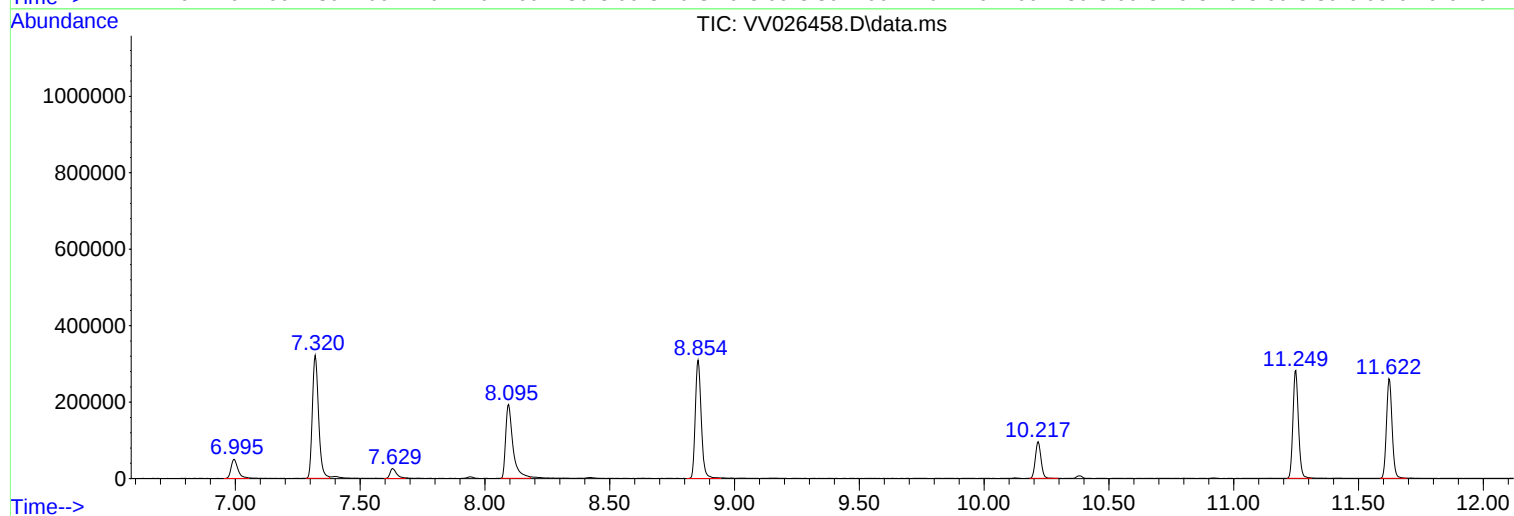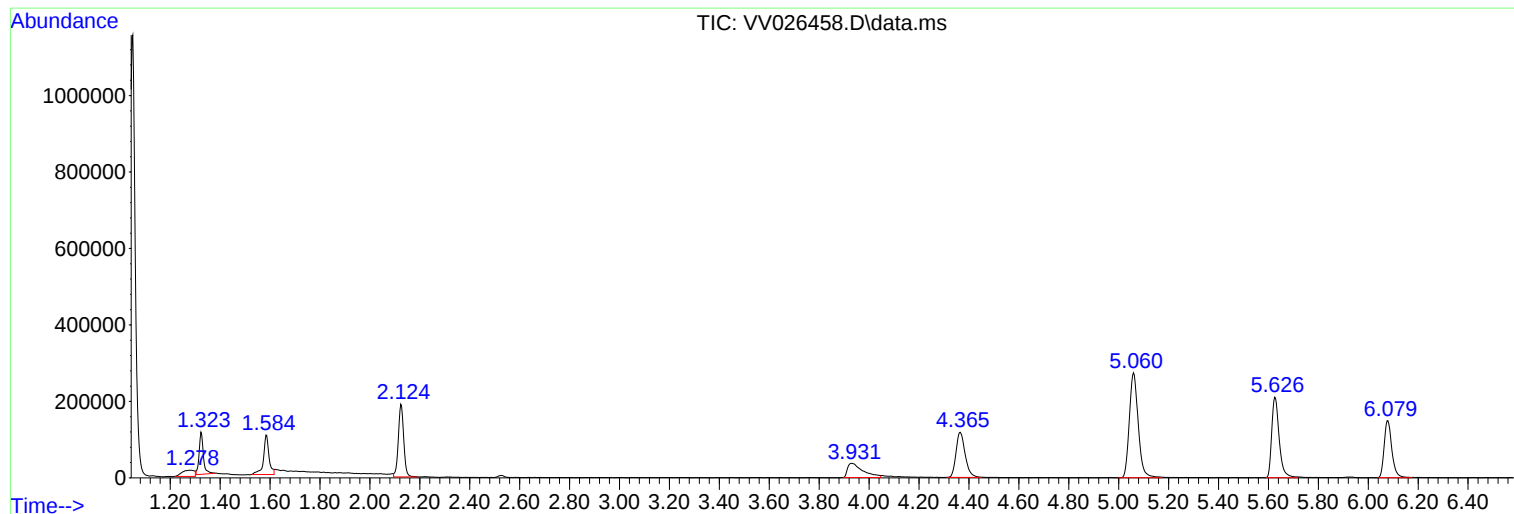

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026458.D
Acq On : 20 Jun 2022 20:13
Operator : SY/MD
Sample : N3318-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Naphthalene, 2-ethenyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.480	1.97 ug/L	170113	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acenaphthene	154	C12H10	000083-32-9	93
2			Acenaphthene	154	C12H10	000083-32-9	89
3			Naphthalene, 2-ethenyl-	154	C12H10	000827-54-3	68
4			Acenaphthene	154	C12H10	000083-32-9	60
5			Acenaphthene	154	C12H10	000083-32-9	59

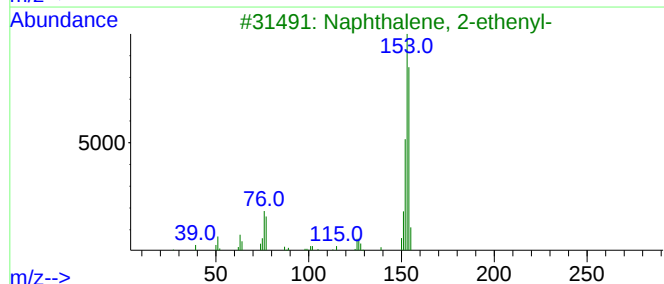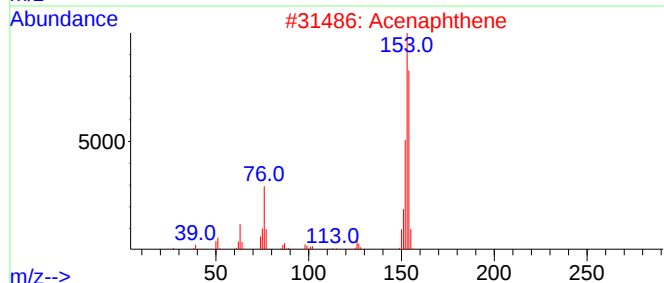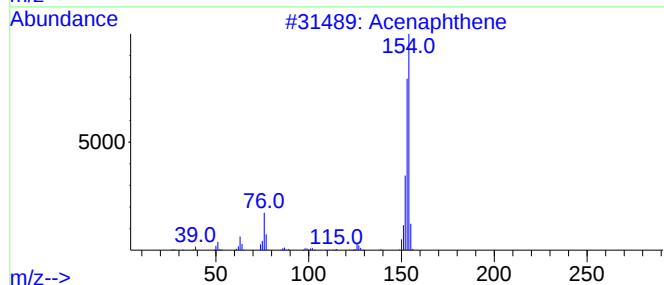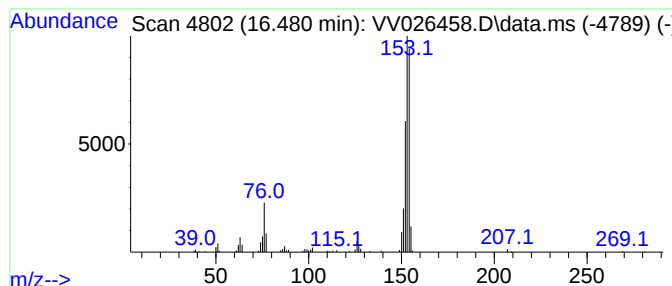

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026458.D
Acq On : 20 Jun 2022 20:13
Operator : SY/MD
Sample : N3318-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Naphthalene, 2-...	16.480	2.0	ug/L	170113	3	11.249	432225	5.0