

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026465.D
 Acq On : 20 Jun 2022 23:00
 Operator : SY/MD
 Sample : N3401-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.259	56	68	69	rBV5	14388	20686	3.02%	0.440%
2	1.323	81	88	102	rVB	108510	120178	17.55%	2.557%
3	1.584	161	169	181	rBV	97752	121660	17.77%	2.589%
4	2.124	326	337	357	rVB	197868	294147	42.96%	6.260%
5	3.931	888	899	915	rBV2	36400	123653	18.06%	2.631%
6	4.362	1017	1033	1057	rBV	121885	303486	44.32%	6.458%
7	5.060	1234	1250	1275	rBV2	280155	684698	100.00%	14.571%
8	5.625	1415	1426	1461	rBV	155245	322376	47.08%	6.860%
9	6.076	1554	1566	1586	rBV	154634	317710	46.40%	6.761%
10	6.995	1841	1852	1877	rBV2	42442	84175	12.29%	1.791%
11	7.320	1942	1953	1970	rBV	320763	566089	82.68%	12.047%
12	7.400	1971	1978	1997	rVB	10064	21603	3.16%	0.460%
13	7.629	2041	2049	2072	rBV	22055	41371	6.04%	0.880%
14	8.095	2183	2194	2228	rBV3	192939	406326	59.34%	8.647%
15	8.854	2419	2430	2456	rBV	230355	382758	55.90%	8.145%
16	10.217	2843	2854	2876	rBV	97350	153538	22.42%	3.267%
17	10.381	2893	2905	2915	rBV3	9364	14690	2.15%	0.313%
18	11.249	3164	3175	3196	rBV	198694	311620	45.51%	6.631%
19	11.622	3280	3291	3315	rBV	254919	408422	59.65%	8.691%




Sum of corrected areas: 4699186

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026465.D
Acq On : 20 Jun 2022 23:00
Operator : SY/MD
Sample : N3401-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

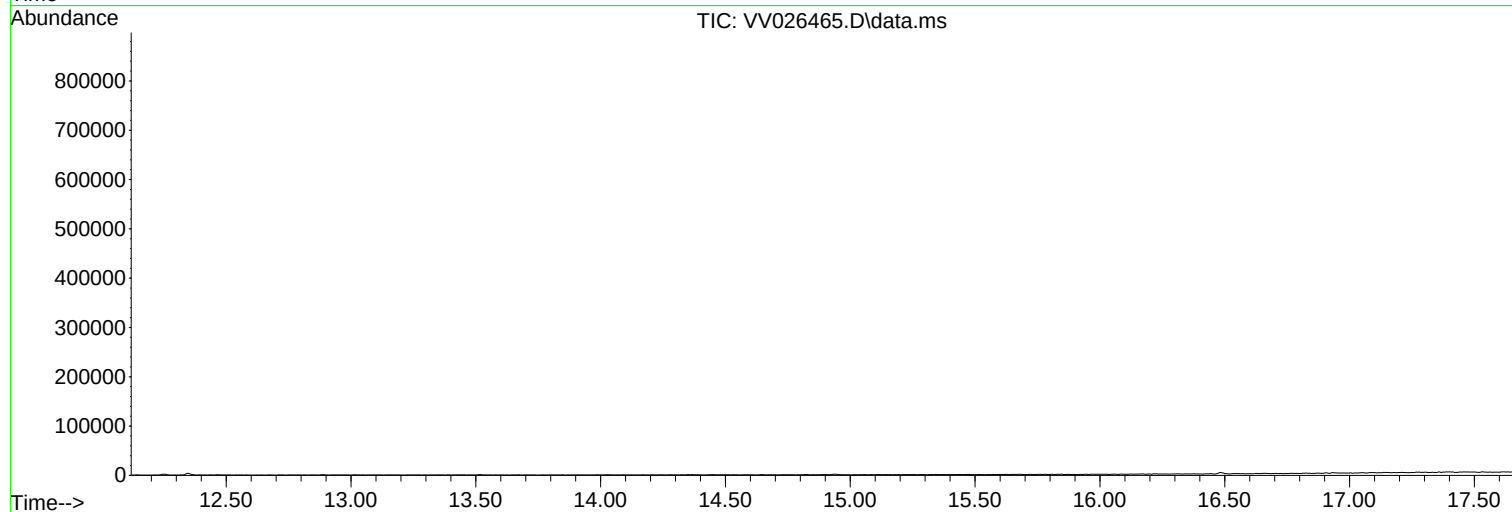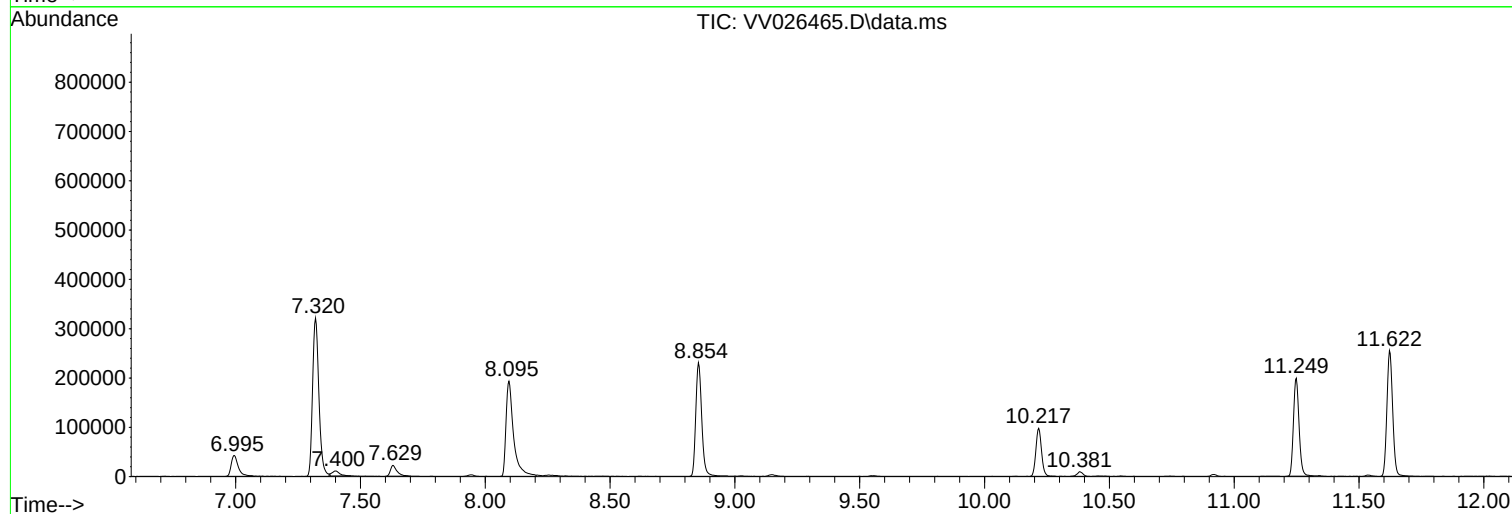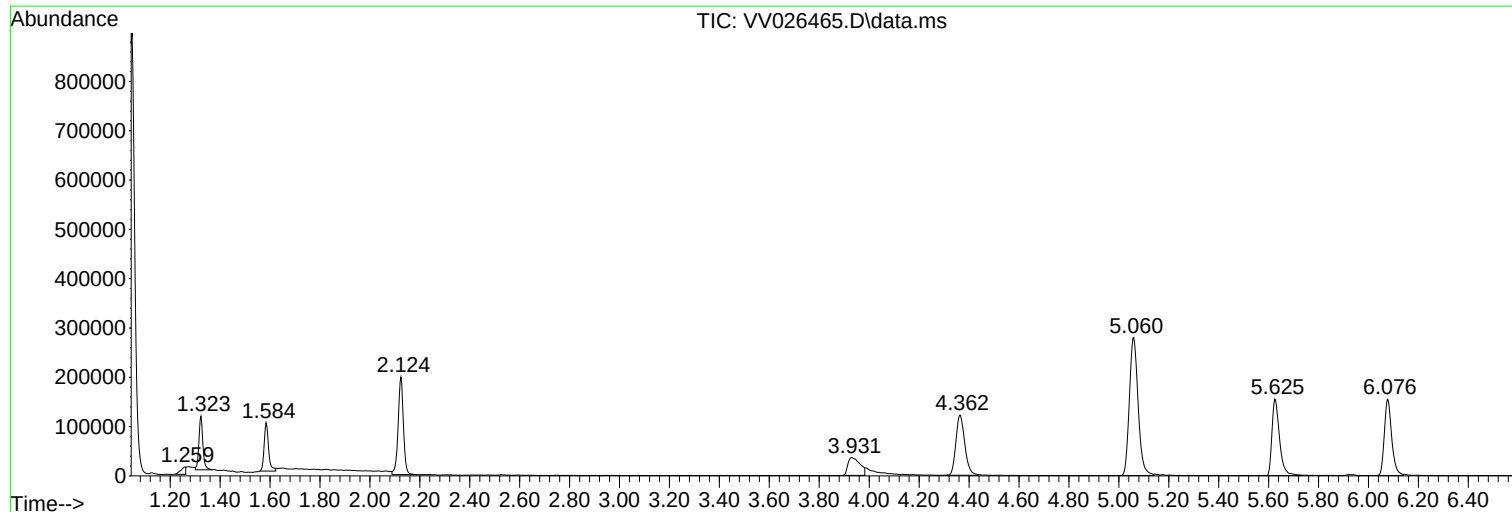

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026465.D
Acq On : 20 Jun 2022 23:00
Operator : SY/MD
Sample : N3401-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026465.D
Acq On : 20 Jun 2022 23:00
Operator : SY/MD
Sample : N3401-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc