

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026466.D
 Acq On : 20 Jun 2022 23:24
 Operator : SY/MD
 Sample : N3401-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	41	rVB2	18111	20865	3.09%	0.381%
2	1.262	54	69	72	rBV3	16495	31583	4.68%	0.576%
3	1.323	80	88	100	rVB	115747	130430	19.32%	2.381%
4	1.433	115	122	130	rVB	39298	44719	6.62%	0.816%
5	1.584	148	169	185	rBV	104052	168701	24.99%	3.079%
6	2.124	327	337	352	rVB	191267	280344	41.53%	5.117%
7	2.311	386	395	408	rVB	21981	33908	5.02%	0.619%
8	2.523	453	461	472	rVB4	4852	8451	1.25%	0.154%
9	3.198	656	671	687	rBV3	7066	14990	2.22%	0.274%
10	3.931	875	899	940	rBV3	44832	210488	31.18%	3.842%
11	4.362	1018	1033	1060	rBV	119064	294948	43.69%	5.383%
12	5.060	1234	1250	1291	rBV2	268467	675116	100.00%	12.322%
13	5.626	1413	1426	1453	rBV	202448	413491	61.25%	7.547%
14	6.076	1552	1566	1589	rBV	148622	306367	45.38%	5.592%
15	6.995	1841	1852	1873	rBV2	41228	79042	11.71%	1.443%
16	7.320	1941	1953	1967	rVV	316948	551037	81.62%	10.058%
17	7.394	1967	1976	1999	rVB	70523	134070	19.86%	2.447%
18	7.632	2039	2050	2066	rBV2	21681	39753	5.89%	0.726%
19	8.095	2183	2194	2229	rBV3	191626	406484	60.21%	7.419%
20	8.854	2419	2430	2453	rBV	296775	491905	72.86%	8.978%
21	9.018	2473	2481	2491	rBV3	7066	11420	1.69%	0.208%
22	9.143	2511	2520	2540	rVB	22933	38666	5.73%	0.706%
23	9.548	2636	2646	2662	rBV2	19003	31390	4.65%	0.573%
24	10.217	2840	2854	2867	rBV	98207	153905	22.80%	2.809%
25	10.381	2887	2905	2918	rBV3	9387	17433	2.58%	0.318%
26	10.452	2918	2927	2931	rBV2	6790	8796	1.30%	0.161%
27	10.915	3061	3071	3085	rBV	19630	29702	4.40%	0.542%
28	11.249	3163	3175	3193	rBV	265238	411601	60.97%	7.513%
29	11.336	3195	3202	3214	rVB3	8387	13381	1.98%	0.244%
30	11.532	3252	3263	3274	rBV9	5895	11609	1.72%	0.212%
31	11.622	3280	3291	3316	rVB	261916	414202	61.35%	7.560%




Sum of corrected areas: 5478797

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026466.D
Acq On : 20 Jun 2022 23:24
Operator : SY/MD
Sample : N3401-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

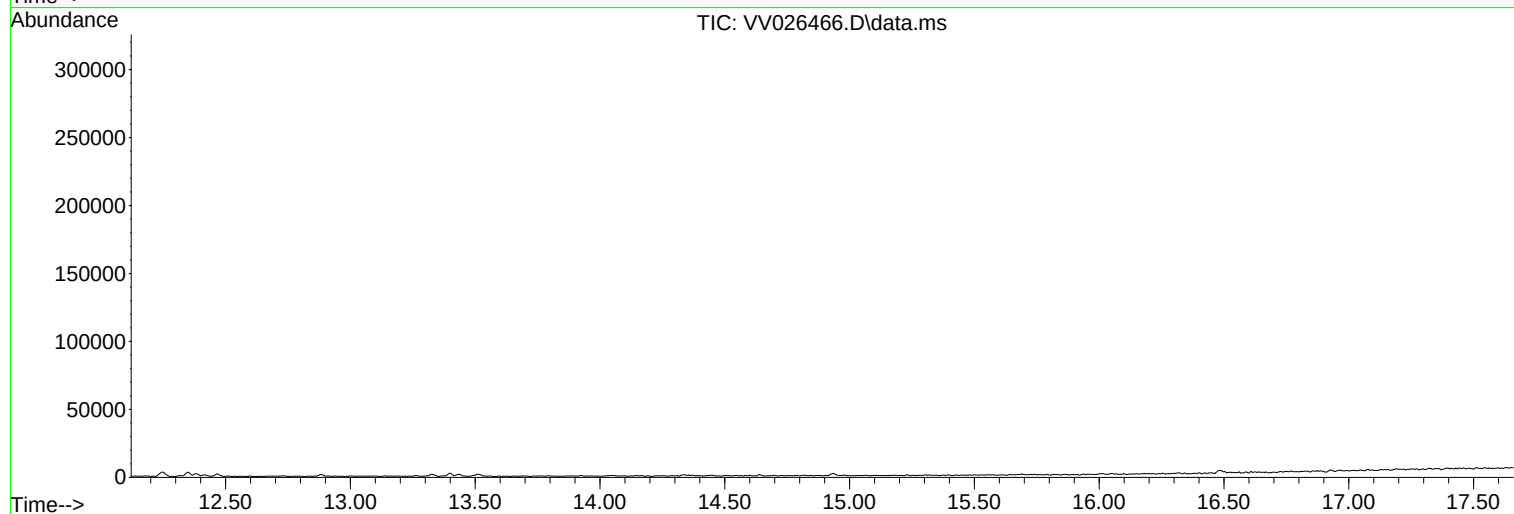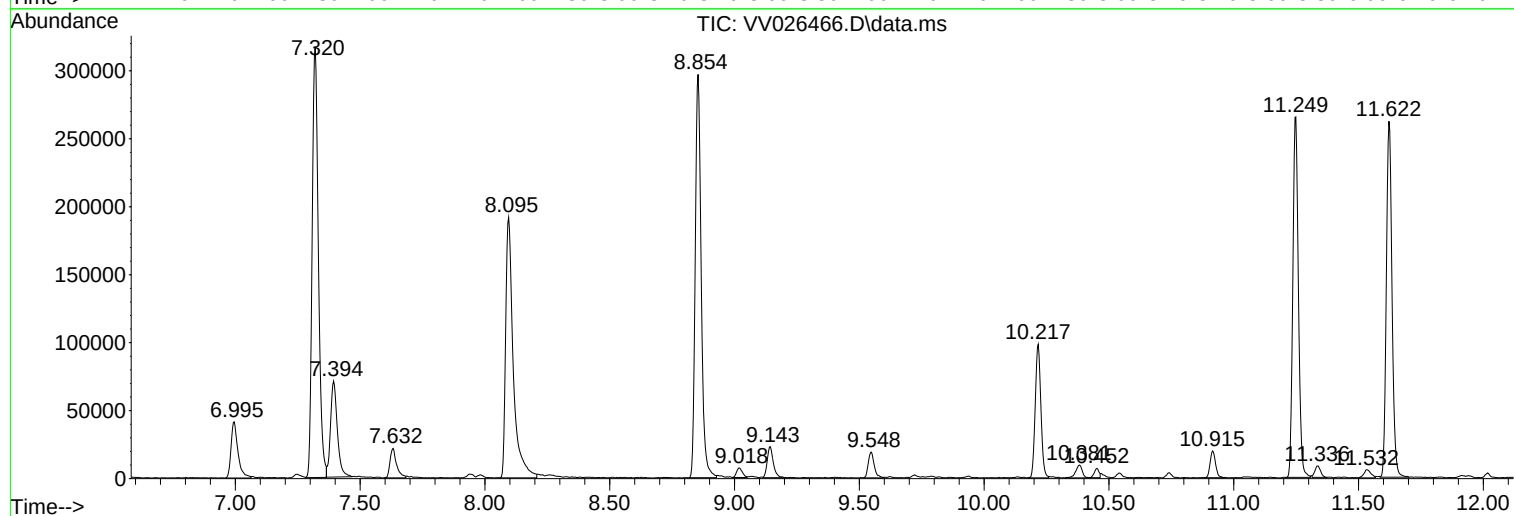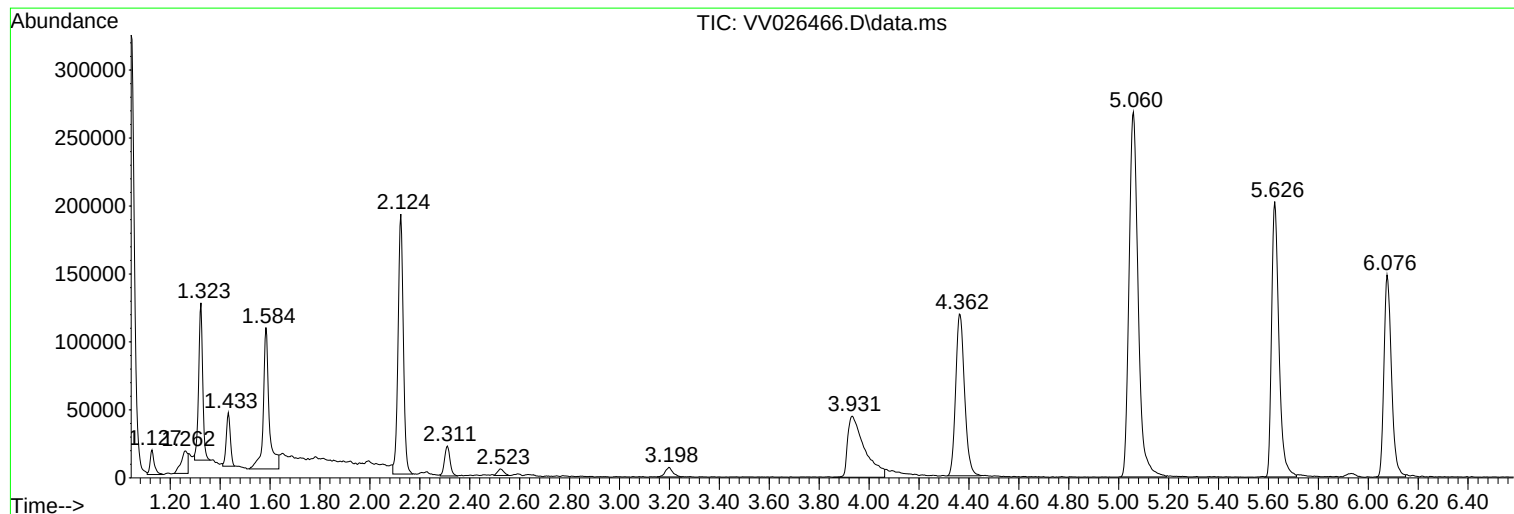

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026466.D
Acq On : 20 Jun 2022 23:24
Operator : SY/MD
Sample : N3401-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026466.D
Acq On : 20 Jun 2022 23:24
Operator : SY/MD
Sample : N3401-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc