

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026467.D
 Acq On : 20 Jun 2022 23:48
 Operator : SY/MD
 Sample : N3401-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.265	54	70	72	rBV4	13092	25605	4.07%	0.562%
2	1.323	82	88	101	rVB	99247	106807	16.99%	2.344%
3	1.584	161	169	180	rBV	94953	115815	18.42%	2.541%
4	2.124	327	337	352	rVB	179900	260481	41.44%	5.715%
5	2.310	387	395	406	rVB	11020	16980	2.70%	0.373%
6	2.523	454	461	471	rVB4	4909	8036	1.28%	0.176%
7	2.593	474	483	496	rVB3	7442	12609	2.01%	0.277%
8	3.934	885	900	931	rBV	34518	149621	23.80%	3.283%
9	4.365	1017	1034	1053	rBV2	114772	284226	45.22%	6.237%
10	5.059	1234	1250	1282	rBV2	251691	628604	100.00%	13.793%
11	5.625	1415	1426	1451	rBV	167069	343560	54.65%	7.538%
12	6.075	1552	1566	1593	rBV	139210	294452	46.84%	6.461%
13	6.995	1841	1852	1876	rBV	37797	73404	11.68%	1.611%
14	7.320	1941	1953	1970	rBV	285844	503467	80.09%	11.047%
15	7.397	1971	1977	1996	rVB	11971	24693	3.93%	0.542%
16	7.632	2039	2050	2069	rBV2	20546	38066	6.06%	0.835%
17	8.095	2184	2194	2233	rBV2	179526	384302	61.14%	8.432%
18	8.854	2418	2430	2460	rBV	250645	415195	66.05%	9.110%
19	9.143	2512	2520	2536	rBV2	8702	14372	2.29%	0.315%
20	10.217	2843	2854	2873	rBV	91657	145592	23.16%	3.195%
21	10.381	2896	2905	2919	rVB4	7405	12083	1.92%	0.265%
22	11.249	3164	3175	3198	rBV	213533	332728	52.93%	7.301%
23	11.622	3280	3291	3309	rBV	228147	366754	58.34%	8.047%




Sum of corrected areas: 4557452

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026467.D
Acq On : 20 Jun 2022 23:48
Operator : SY/MD
Sample : N3401-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

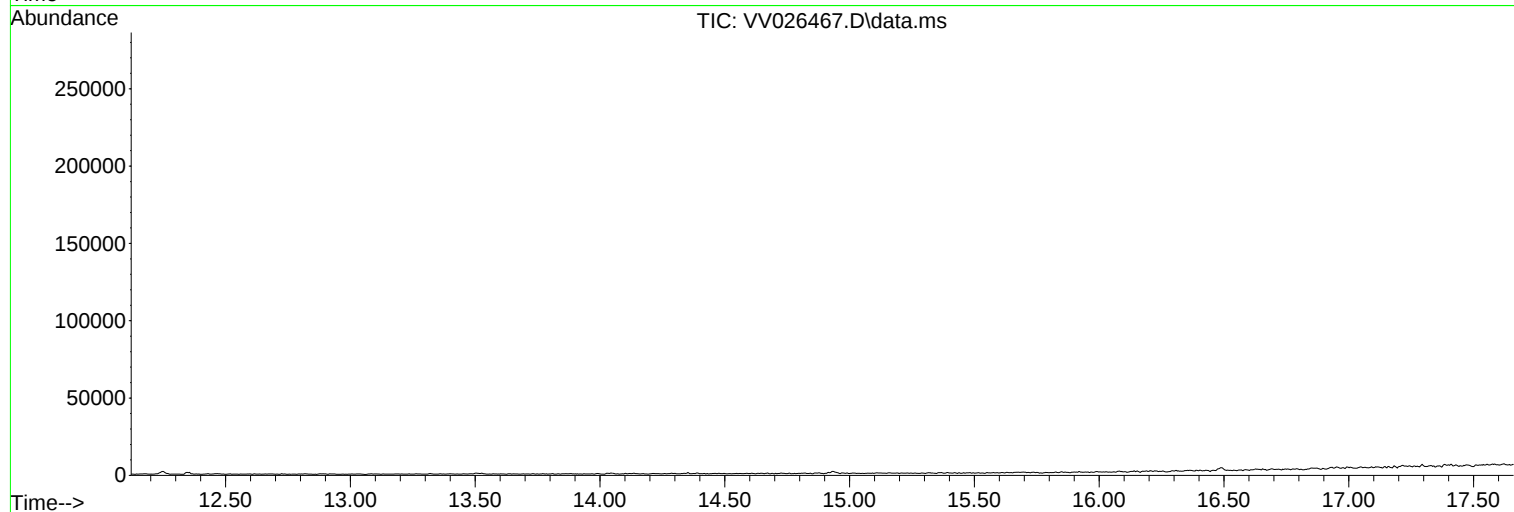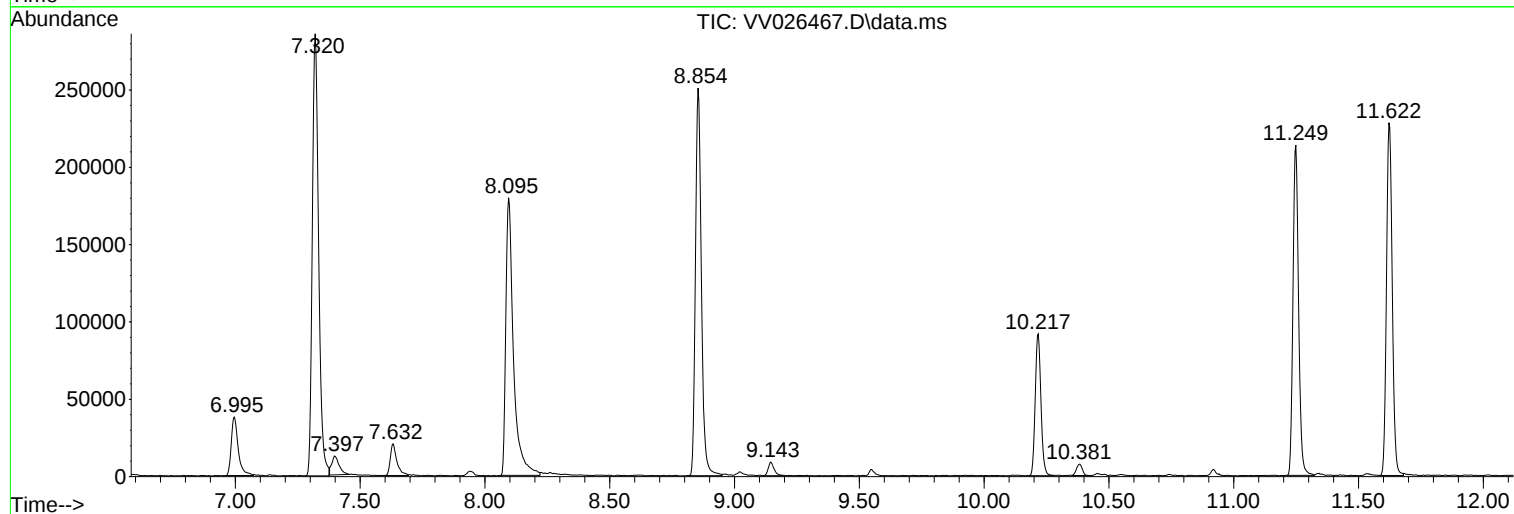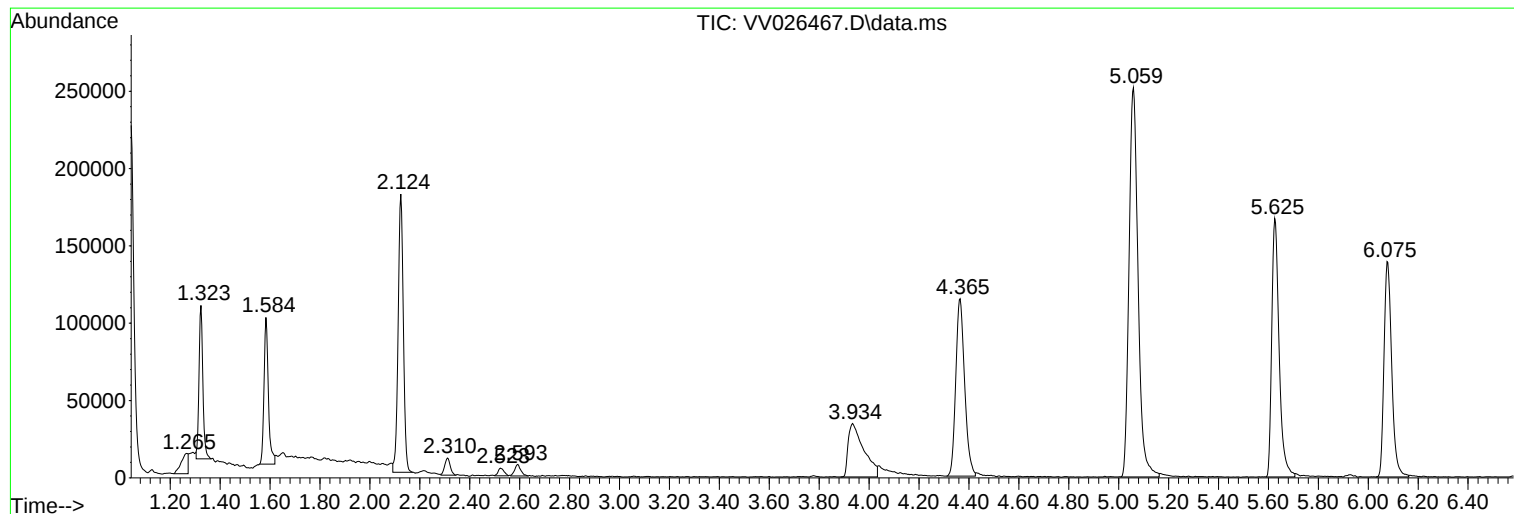

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026467.D
Acq On : 20 Jun 2022 23:48
Operator : SY/MD
Sample : N3401-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026467.D
Acq On : 20 Jun 2022 23:48
Operator : SY/MD
Sample : N3401-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------