

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
 Data File : VV026471.D
 Acq On : 21 Jun 2022 01:23
 Operator : SY/MD
 Sample : N3345-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.272	55	72	77	rBV2	14009	36760	6.12%	0.737%
2	1.323	81	88	109	rVB	98884	123462	20.57%	2.476%
3	1.587	162	170	183	rBV	84559	107924	17.98%	2.164%
4	2.124	328	337	351	rVB	170572	251278	41.87%	5.039%
5	2.310	388	395	408	rVB	7460	12346	2.06%	0.248%
6	3.934	889	900	942	rBV4	39422	167234	27.86%	3.353%
7	4.368	1019	1035	1074	rVB4	126668	406476	67.73%	8.151%
8	5.060	1233	1250	1278	rBV2	244047	600186	100.00%	12.035%
9	5.625	1414	1426	1459	rBV	196546	403128	67.17%	8.084%
10	5.931	1509	1521	1536	rBV4	15017	32153	5.36%	0.645%
11	6.079	1549	1567	1601	rBV	134762	286068	47.66%	5.736%
12	6.590	1713	1726	1738	rBV3	5930	12491	2.08%	0.250%
13	6.992	1842	1851	1869	rBV2	44439	84393	14.06%	1.692%
14	7.320	1941	1953	1970	rBV	277175	490223	81.68%	9.830%
15	7.397	1971	1977	1989	rVB	11405	22071	3.68%	0.443%
16	7.629	2041	2049	2066	rBV2	24047	44819	7.47%	0.899%
17	7.979	2148	2158	2184	rVB	80650	138044	23.00%	2.768%
18	8.095	2184	2194	2230	rBV	175289	366575	61.08%	7.351%
19	8.854	2416	2430	2453	rBV	288690	478041	79.65%	9.586%
20	9.153	2510	2523	2534	rBV4	3695	7116	1.19%	0.143%
21	10.217	2840	2854	2872	rBV	87235	142021	23.66%	2.848%
22	10.381	2895	2905	2917	rBV5	6310	9559	1.59%	0.192%
23	11.249	3163	3175	3197	rBV	255359	400598	66.75%	8.033%
24	11.622	3280	3291	3308	rBV	228298	364050	60.66%	7.300%




Sum of corrected areas: 4987016

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026471.D
Acq On : 21 Jun 2022 01:23
Operator : SY/MD
Sample : N3345-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

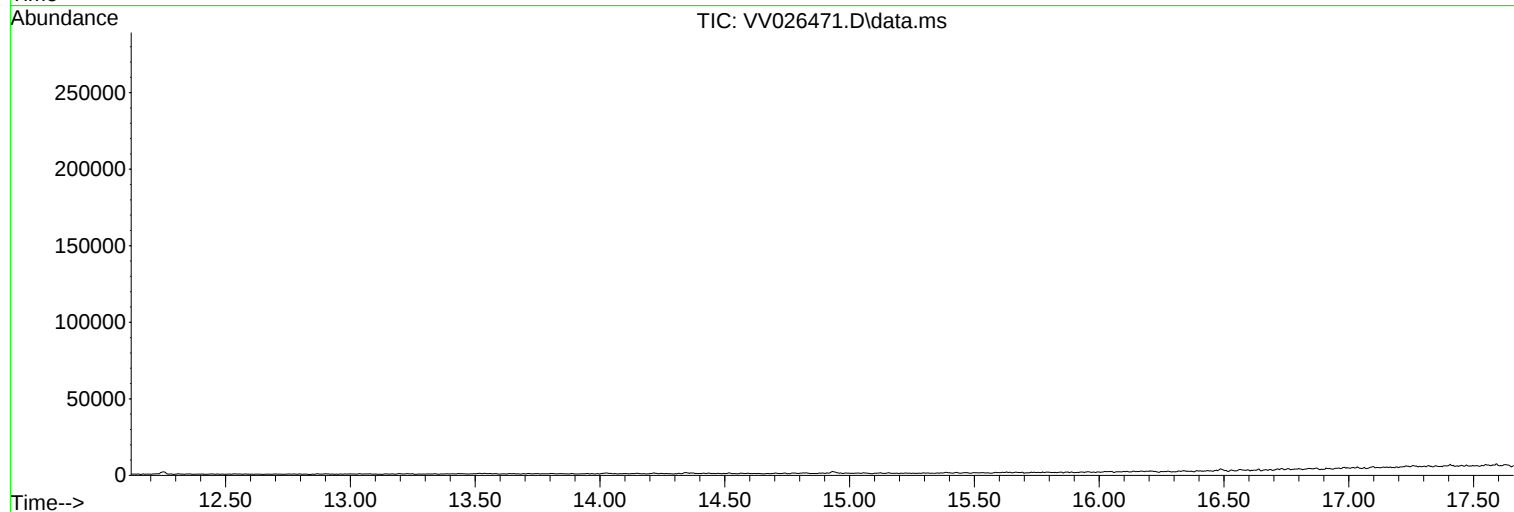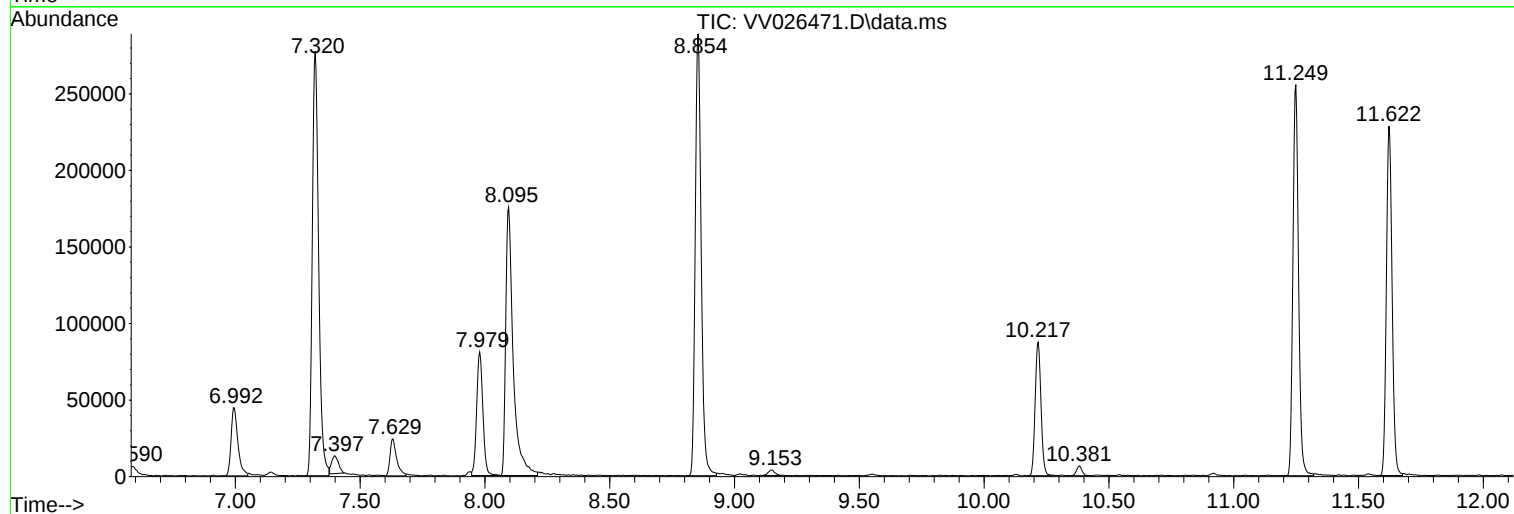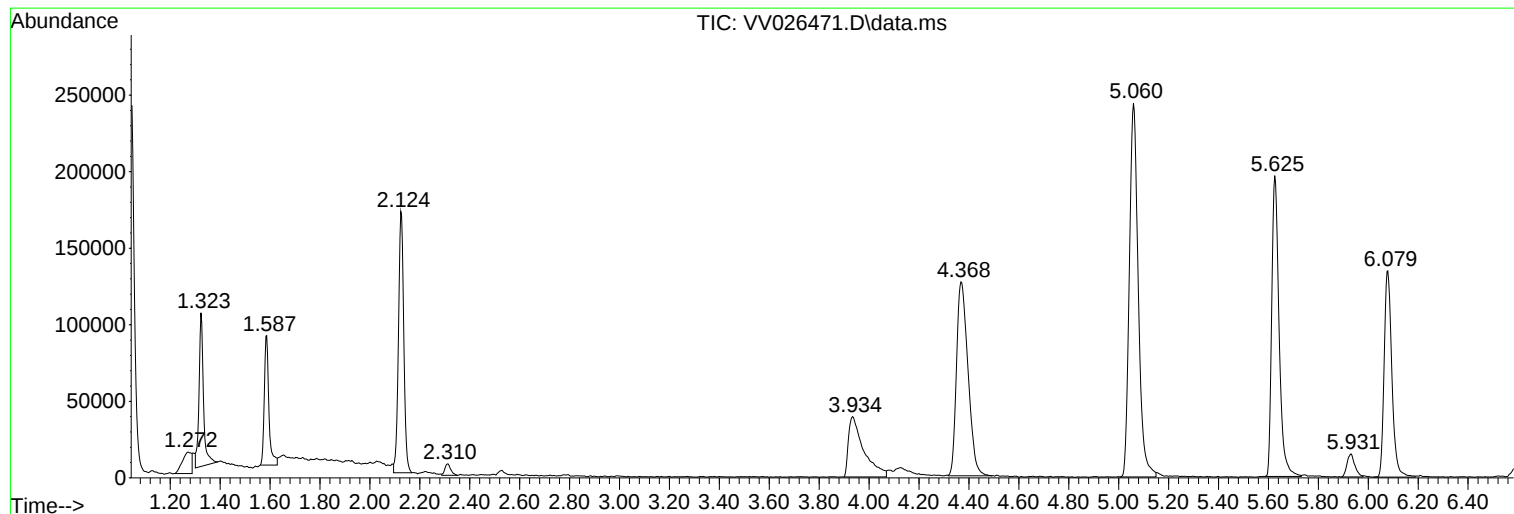

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026471.D
Acq On : 21 Jun 2022 01:23
Operator : SY/MD
Sample : N3345-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062022\
Data File : VV026471.D
Acq On : 21 Jun 2022 01:23
Operator : SY/MD
Sample : N3345-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc