

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062024\
 Data File : VV036156.D
 Acq On : 20 Jun 2024 11:53
 Operator : SY/MD
 Sample : P2909-12RE
 Misc : 5.11g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4CP1RE

Quant Time: Jun 21 01:47:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 20 05:02:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	312031	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	152325	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	29048	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	139231	24.270	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.080%
7) Chloroethane-d5	1.526	69	118511	25.908	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.640%
11) 1,1-Dichloroethene-d2	2.050	65	53717	21.034	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.120%
21) 2-Butanone-d5	0.000	46	0d	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
24) Chloroform-d	4.243	84	185351	18.684	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.720%
26) 1,2-Dichloroethane-d4	4.937	65	95181	18.300	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.200%
32) Benzene-d6	4.957	84	258398	28.538	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	114.160%
36) 1,2-Dichloropropane-d6	5.986	67	106201	37.245	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	149.000%#
41) Toluene-d8	7.243	98	139795	17.498	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.000%
43) trans-1,3-Dichloroprop...	0.000	79	0d	0.000	ug/L	
Spiked Amount	25.000	Range	30 - 135	Recovery	=	0.000%#
47) 2-Hexanone-d5	0.000	63	0d	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
56) 1,1,2,2-Tetrachloroeth...	10.153	84	46219	21.692	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.760%
66) 1,2-Dichlorobenzene-d4	11.564	152	17242	16.186	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	64.760%#
Target Compounds						
					Qvalue	
13) Acetone	2.127	43	16123	7.864	ug/L	# 43
16) Methylene chloride	2.442	84	19210	2.721	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062024\
Data File : VV036156.D
Acq On : 20 Jun 2024 11:53
Operator : SY/MD
Sample : P2909-12RE
Misc : 5.11g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4CP1RE

Quant Time: Jun 21 01:47:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 20 05:02:48 2024
Response via : Initial Calibration

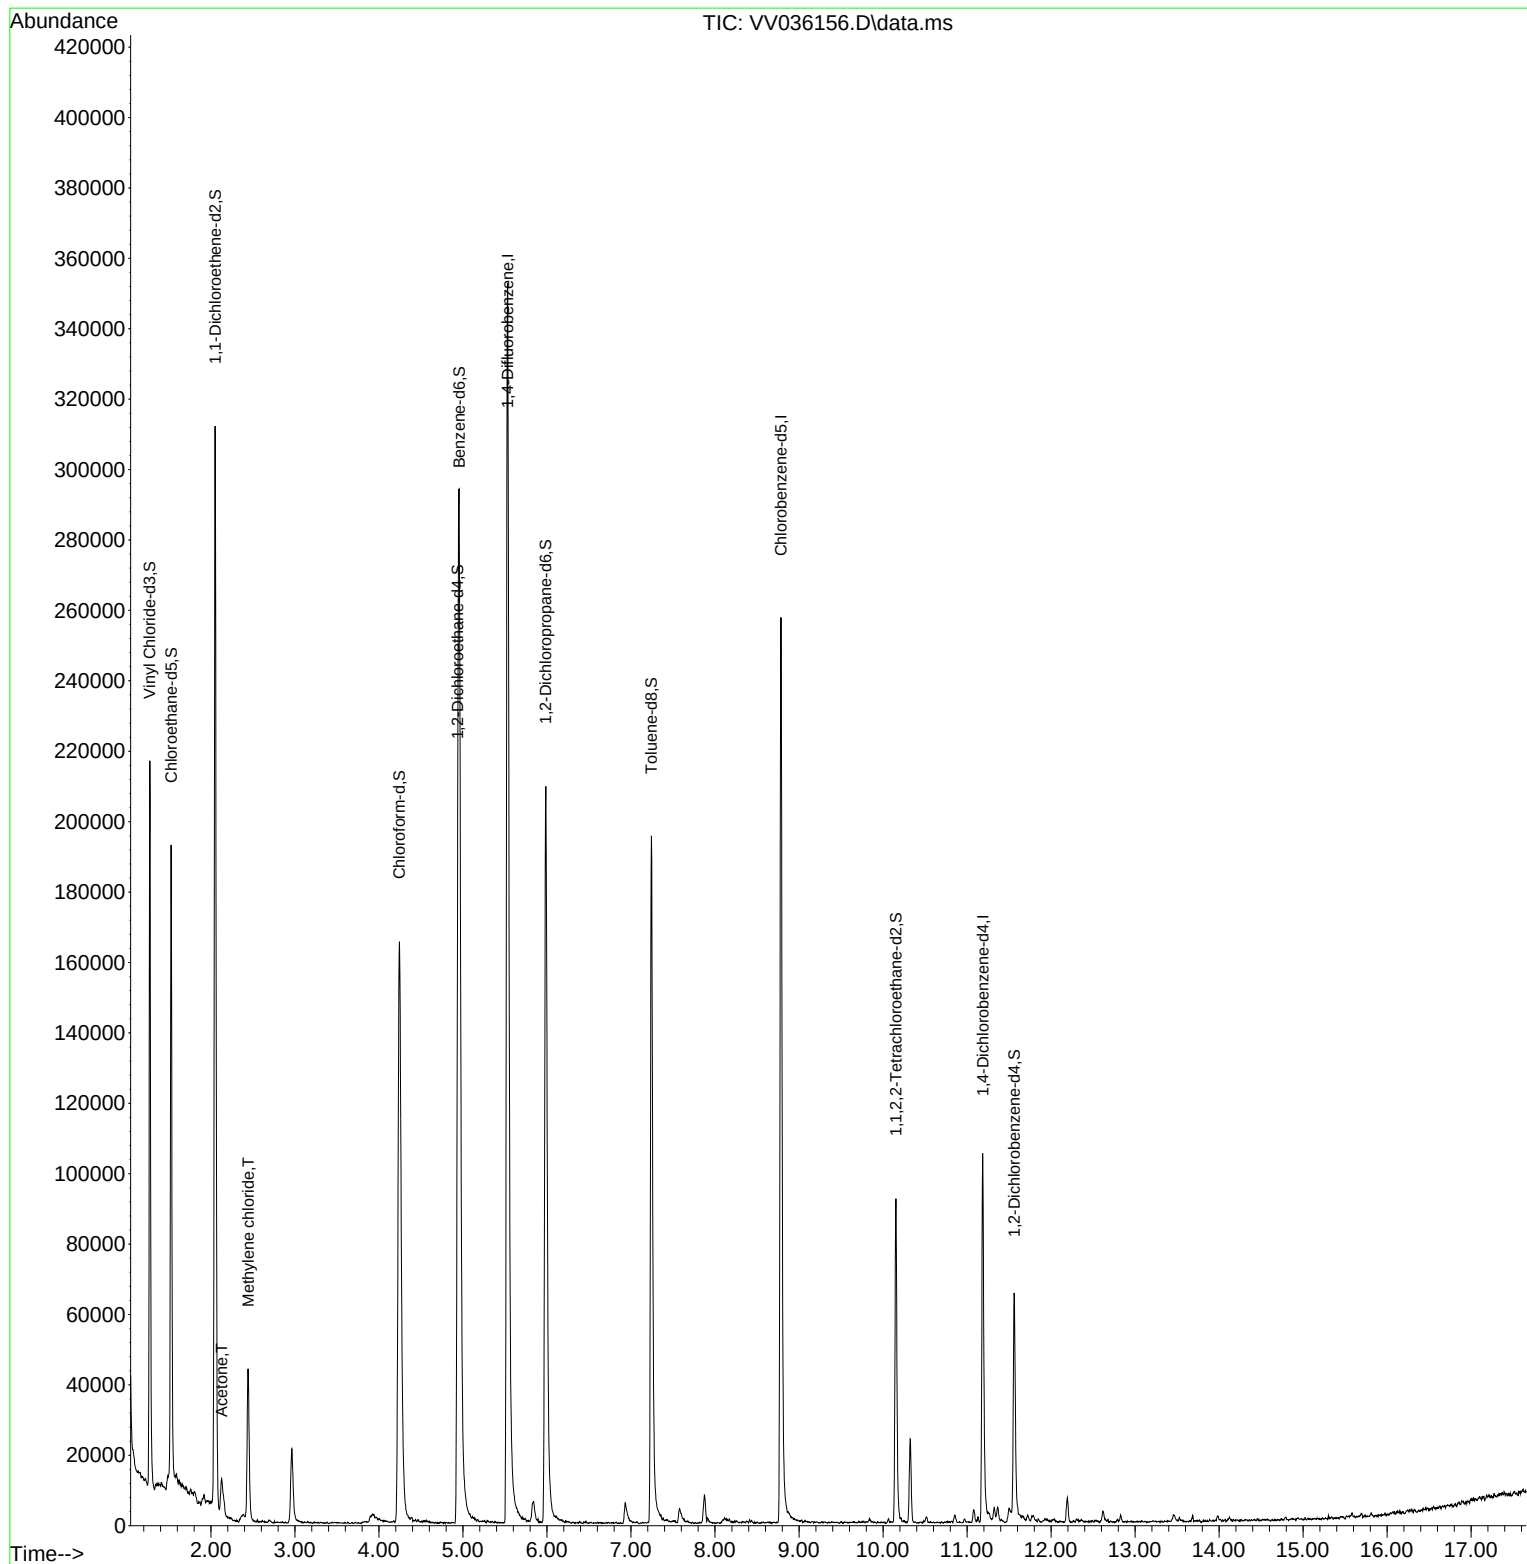

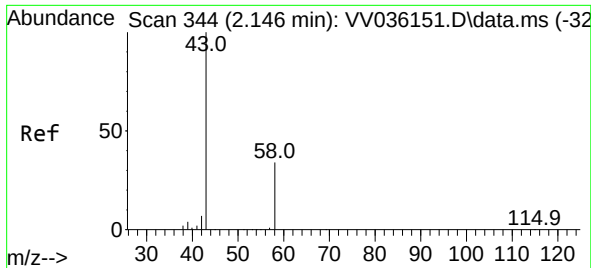

#13

Acetone

Concen: 7.864 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.019 min

Lab File: VV036156.D

Acq: 20 Jun 2024 11:53

Instrument :

MSVOA_V

ClientSampleId :





A4CP1RE

Tgt Ion: 43 Resp: 16123

Ion Ratio Lower Upper

43 100

58 34.2 0.0 24.2#

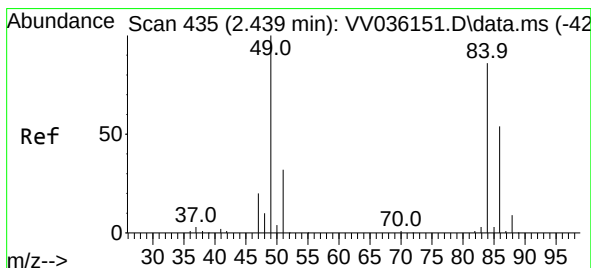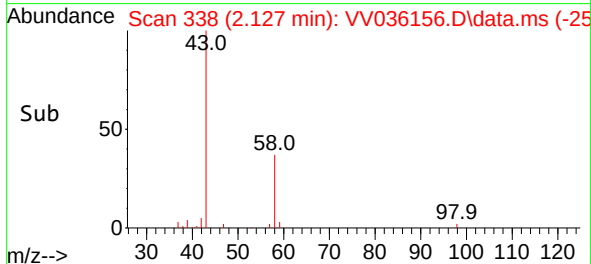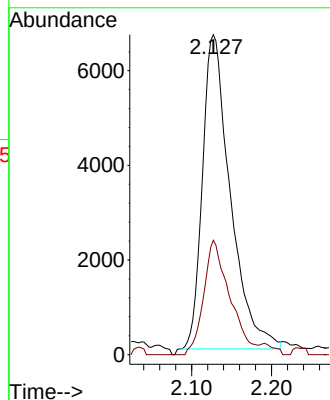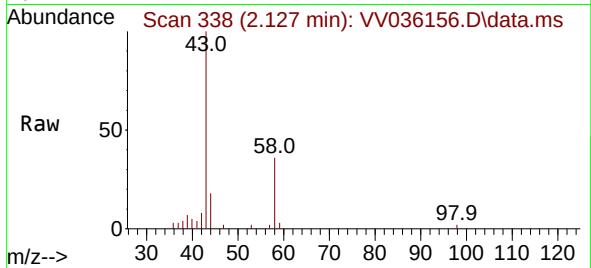

#16

Methylene chloride

Concen: 2.721 ug/L

RT: 2.442 min Scan# 436

Delta R.T. 0.003 min

Lab File: VV036156.D

Acq: 20 Jun 2024 11:53

Tgt Ion: 84 Resp: 19210

Ion Ratio Lower Upper

84 100

86 64.6 44.6 82.8

49 110.6 81.1 150.5

