

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062024\
 Data File : VW036167.D
 Acq On : 20 Jun 2024 16:39
 Operator : SY/MD
 Sample : P2873-21RE
 Misc : 5.04g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COSLORE

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 06/22/2024
 Supervised By :Semsettin Yesilyurt 06/22/2024

Quant Time: Jun 21 01:48:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 20 05:02:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	336419	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	328098	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	106065	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	145971	23.601	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	94.400%		
7) Chloroethane-d5	1.526	69	118860	24.101	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.400%		
11) 1,1-Dichloroethene-d2	2.050	65	58553	21.265	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	85.080%		
21) 2-Butanone-d5	3.831	46	54259m	38.235	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	76.480%		
24) Chloroform-d	4.243	84	245173	22.923	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.680%		
26) 1,2-Dichloroethane-d4	4.937	65	137529	24.525	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	98.080%		
32) Benzene-d6	4.953	84	459095	23.540	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.160%		
36) 1,2-Dichloropropane-d6	5.986	67	150350	24.480	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.920%		
41) Toluene-d8	7.243	98	365583	21.245	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.960%		
43) trans-1,3-Dichloroprop...	7.555	79	54187	21.518	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.080%		
47) 2-Hexanone-d5	8.031	63	33009	39.669	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.340%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	107453	23.413	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.640%		
66) 1,2-Dichlorobenzene-d4	11.558	152	91474	23.518	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.080%		
Target Compounds						
					Qvalue	
13) Acetone	2.153	43	18067	8.173	ug/L #	61
14) Carbon disulfide	2.233	76	85873	4.590	ug/L	100
16) Methylene chloride	2.442	84	38940	5.115	ug/L	99
46) Tetrachloroethene	7.902	164	206241	42.877	ug/L	98
53) m,p-Xylene	9.085	106	3348	0.380	ug/L	90
63) 1,2,4-Trimethylbenzene	10.854	105	5375	0.506	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062024\
Data File : VV036167.D
Acq On : 20 Jun 2024 16:39
Operator : SY/MD
Sample : P2873-21RE
Misc : 5.04g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 20 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0SL0RE

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/22/2024
Supervised By :Semsettin Yesilyurt 06/22/2024

Quant Time: Jun 21 01:48:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 20 05:02:48 2024
Response via : Initial Calibration

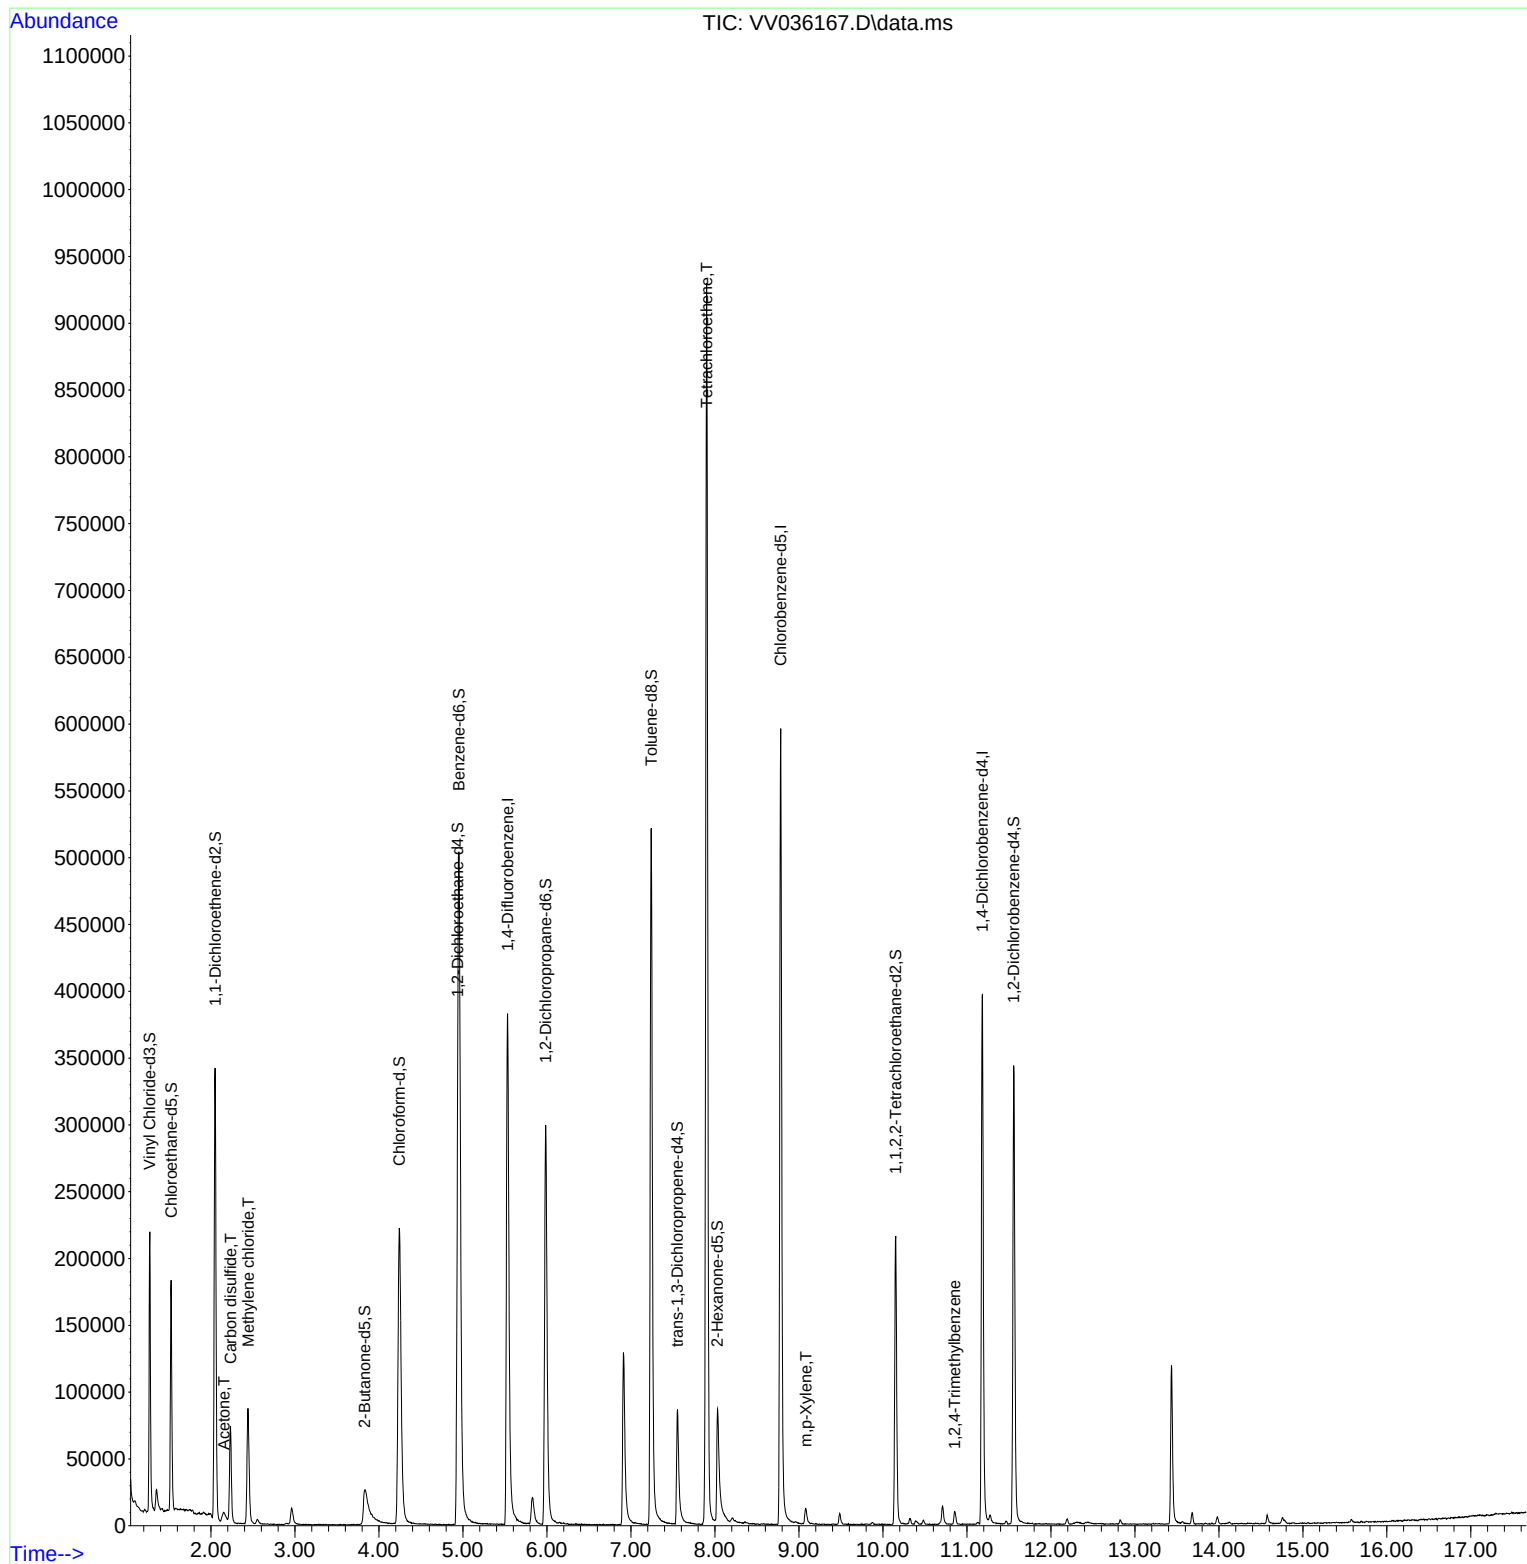

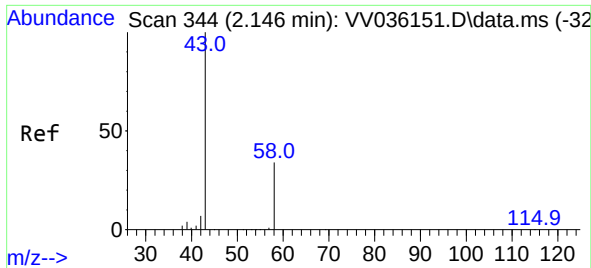





#13
Acetone
Concen: 8.173 ug/L
RT: 2.153 min Scan# 344
Delta R.T. 0.007 min
Lab File: VV036167.D
Acq: 20 Jun 2024 16:39

Instrument :
MSVOA_V
ClientSampleId :
COSLORE

Tgt Ion: 43 Resp: 1806
Ion Ratio Lower Upper
43 100
58 27.2 0.0 24.2




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 06/22/2024
Supervised By :Semsettin Yesilyurt 06/22/2024

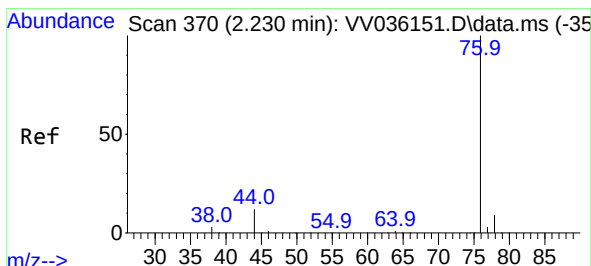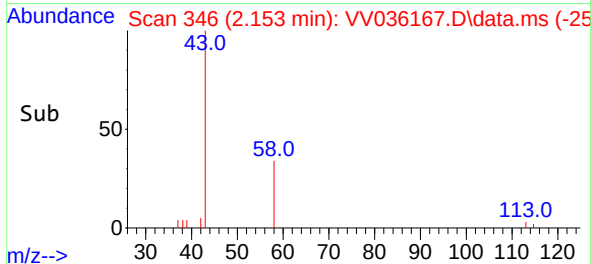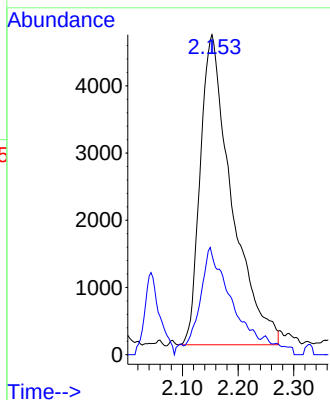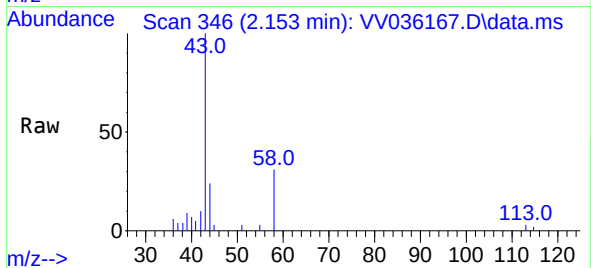

#14
Carbon disulfide
Concen: 4.590 ug/L
RT: 2.233 min Scan# 371
Delta R.T. 0.003 min
Lab File: VV036167.D
Acq: 20 Jun 2024 16:39


Tgt Ion: 76 Resp: 85873
Ion Ratio Lower Upper
76 100
78 9.3 7.4 11.2

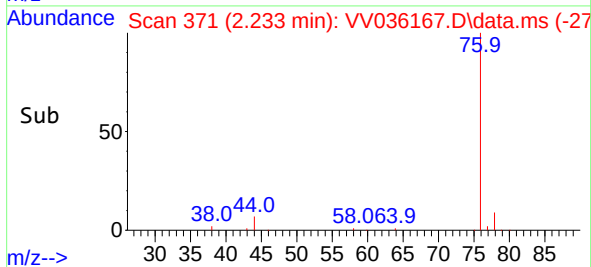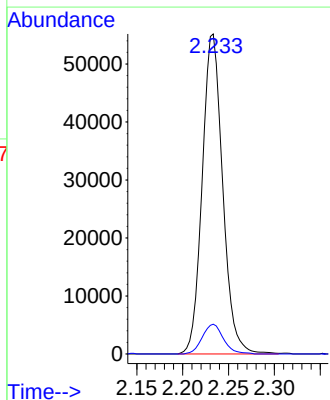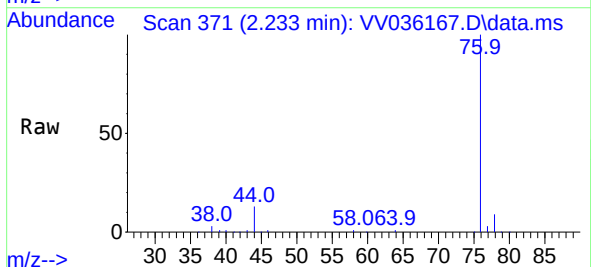

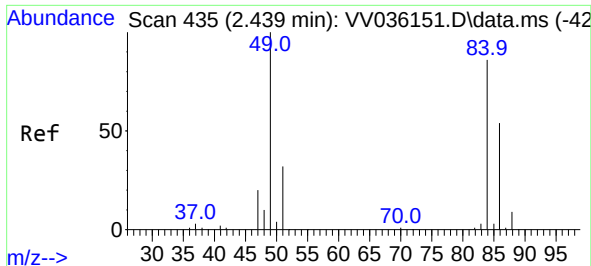

#16
Methylene chloride
Concen: 5.115 ug/L
RT: 2.442 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV036167.D
Acq: 20 Jun 2024 16:39




Instrument :
MSVOA_V
ClientSampleId :
COSLORE

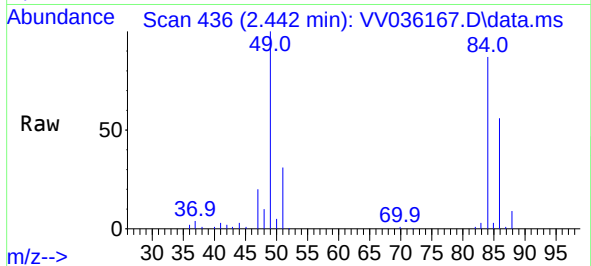

Tgt Ion: 84 Resp: 38940
Ion Ratio Lower Upper
84 100
86 64.7 44.6 82.8
49 115.2 81.1 150.5




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 06/22/2024
Supervised By :Semsettin Yesilyurt 06/22/2024

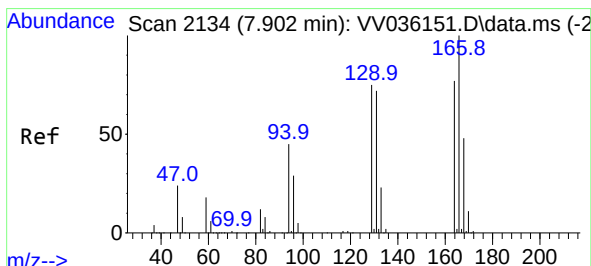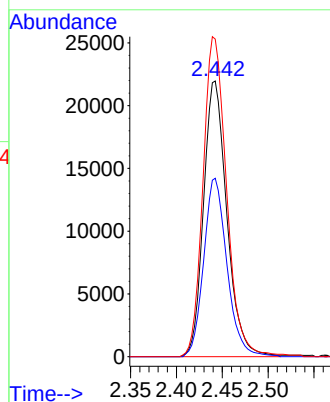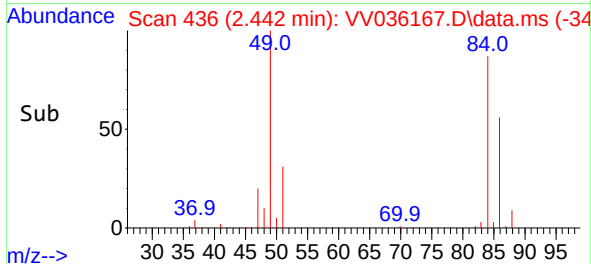

#46
Tetrachloroethene
Concen: 42.877 ug/L
RT: 7.902 min Scan# 2134
Delta R.T. 0.000 min
Lab File: VV036167.D
Acq: 20 Jun 2024 16:39

Tgt Ion:164 Resp: 206241
Ion Ratio Lower Upper
164 100
129 95.6 64.6 120.0
131 90.7 63.2 117.4
166 126.1 89.5 166.3

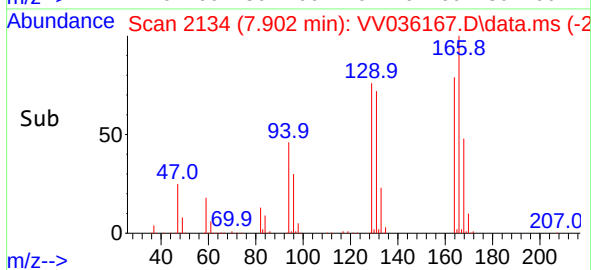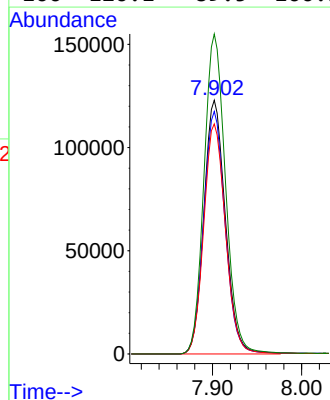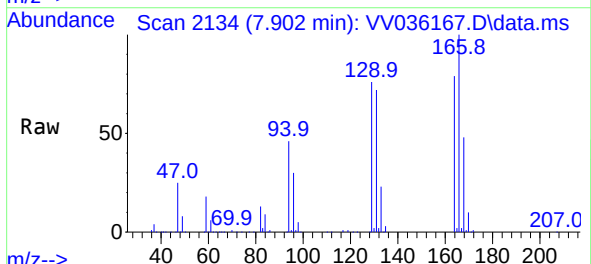

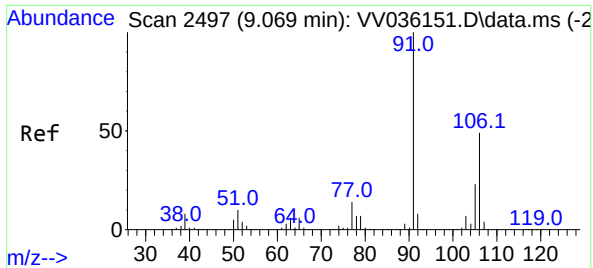





#53
m,p-Xylene
Concen: 0.380 ug/L
RT: 9.085 min Scan# 2106
Delta R.T. 0.016 min
Lab File: VV036167.D
Acq: 20 Jun 2024 16:39

Instrument :
MSVOA_V
ClientSampleId :
COSLORE

Tgt Ion:106 Resp: 3348
Ion Ratio Lower Upper
106 100
91 220.2 143.1 265.9

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/22/2024
Supervised By :Semsettin Yesilyurt 06/22/2024

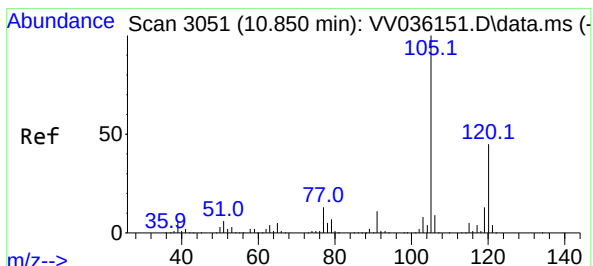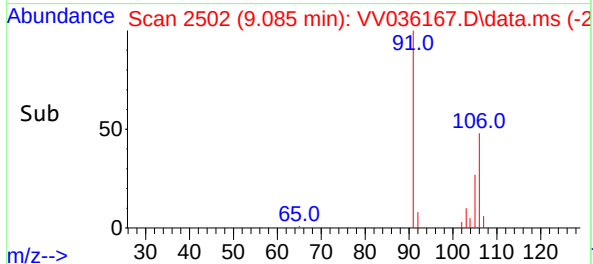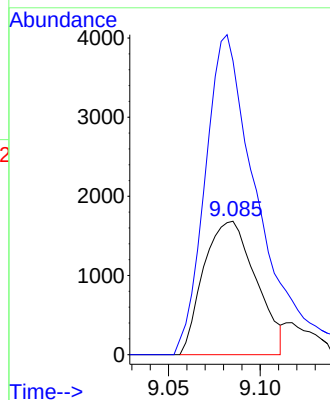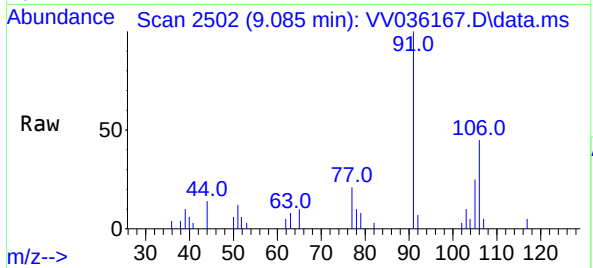

#63
1,2,4-Trimethylbenzene
Concen: 0.506 ug/L
RT: 10.854 min Scan# 3052
Delta R.T. 0.003 min
Lab File: VV036167.D
Acq: 20 Jun 2024 16:39

Tgt Ion:105 Resp: 5375
Ion Ratio Lower Upper
105 100
120 46.4 36.2 54.4

