

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062118\
 Data File : VV006392.D
 Acq On : 21 Jun 2018 14:17
 Operator : SY/MD
 Sample : J3553-05
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KJ3

Quant Time: Jun 22 01:43:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 22 01:25:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	312897	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	283581	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	126435	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	75418	4.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.20%
7) Chloroethane-d5	1.58	69	66354	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.00%
11) 1,1-Dichloroethene-d2	2.14	63	131538	3.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.20%
20) 2-Butanone-d5	3.96	46	219883	60.60	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.20%
24) Chloroform-d	4.41	84	152720	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.09	65	79737	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
32) Benzene-d6	5.11	84	323560	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.12	67	101236	4.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.80%
41) Toluene-d8	7.37	98	282613	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	7.67	79	30258	3.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.00%
46) 2-Hexanone-d5	8.14	63	165806	41.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.78%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	63275	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	106881	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds						Ovalue
12) 1,1-Dichloroethene	2.15	96	51081	2.84	ug/L	93
13) Acetone	2.21	43	17604	8.95	ug/L	89
21) 2-Butanone	4.05	43	14959	4.18	ug/L	91
22) cis-1,2-Dichloroethene	3.97	96	17935	0.85	ug/L #	93
29) 1,1,1-Trichloroethane	4.67	97	15704	0.50	ug/L	97
34) Trichloroethene	5.97	95	94388	4.42	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062118\
Data File : VV006392.D
Acq On : 21 Jun 2018 14:17
Operator : SY/MD
Sample : J3553-05
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KJ3

Quant Time: Jun 22 01:43:46 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 22 01:25:25 2018
Response via : Initial Calibration




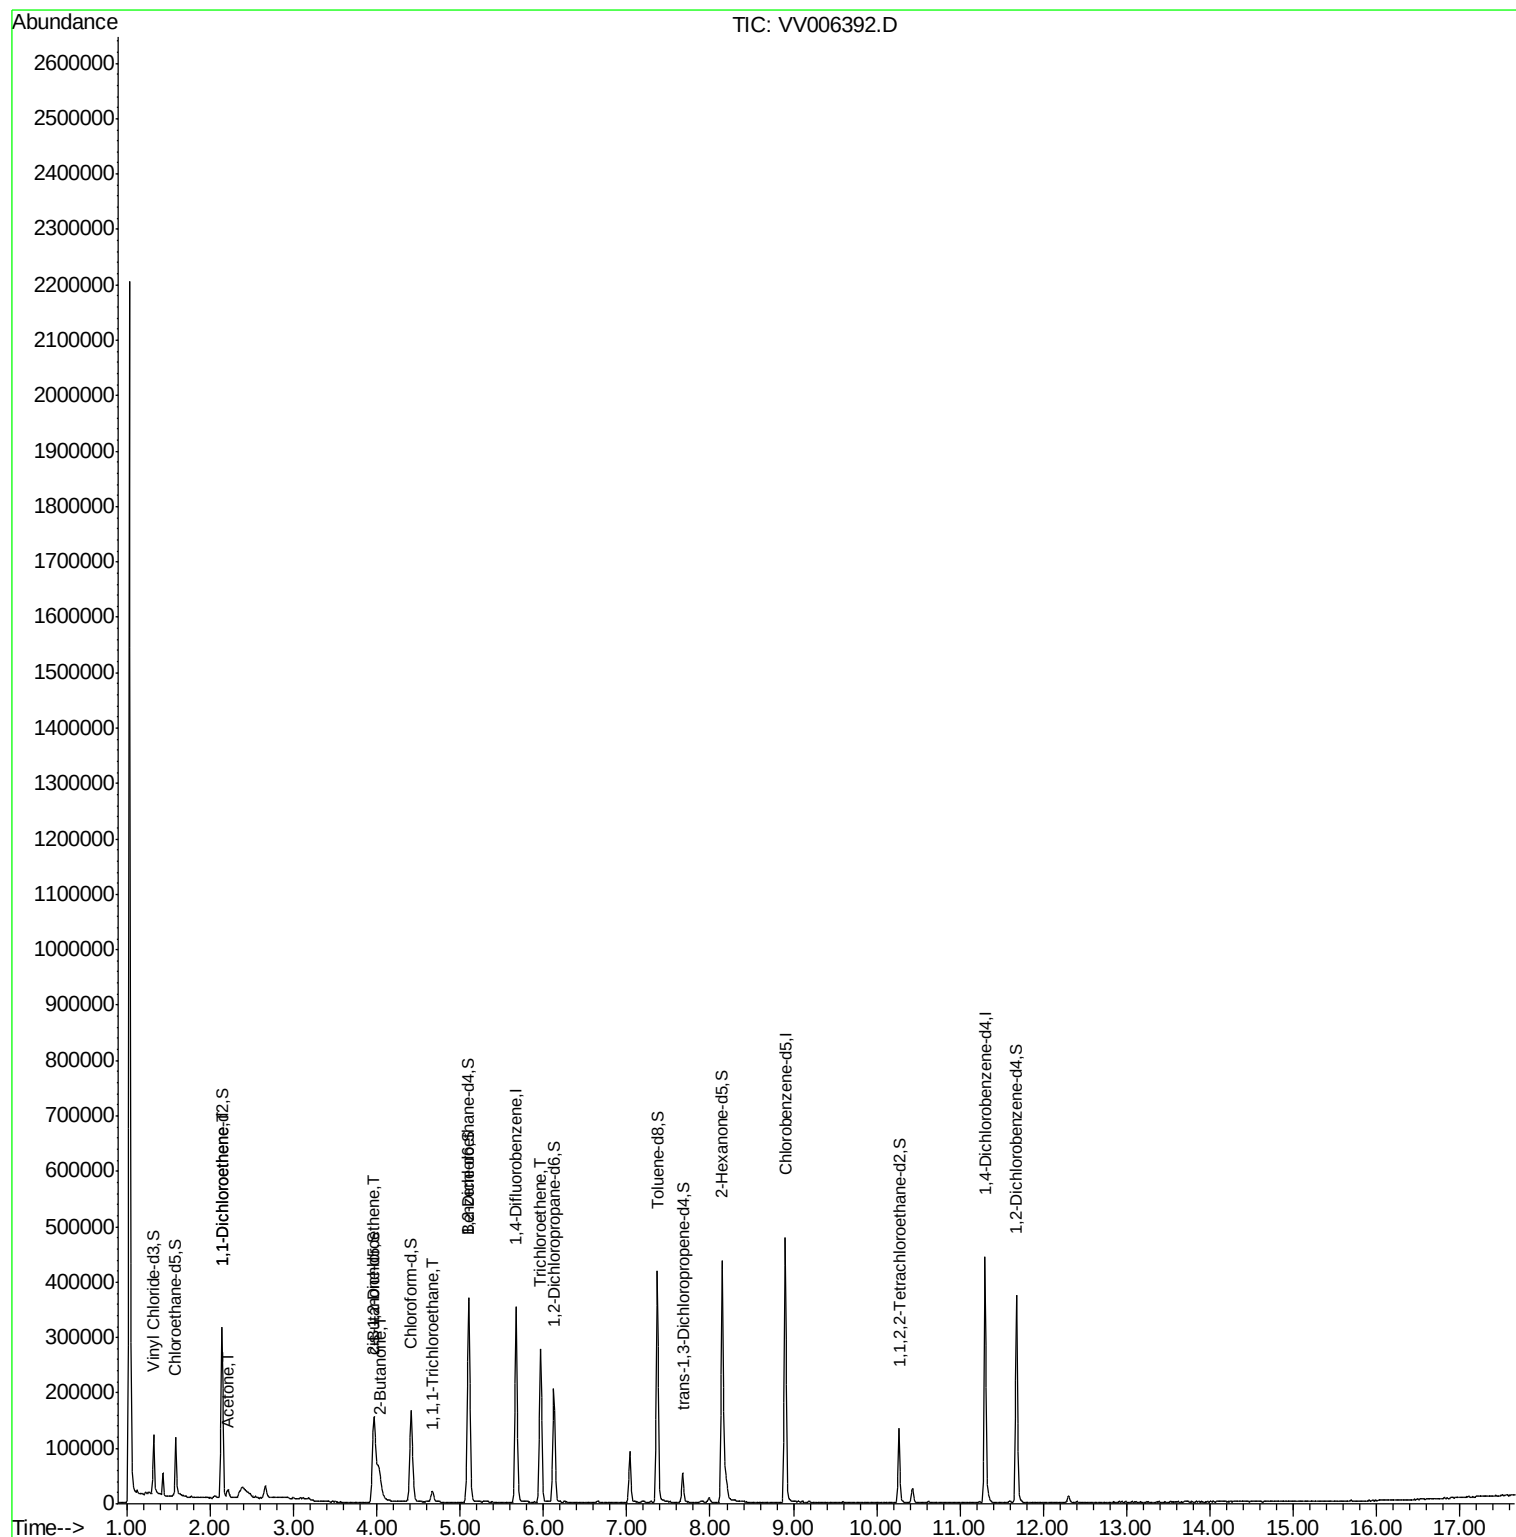


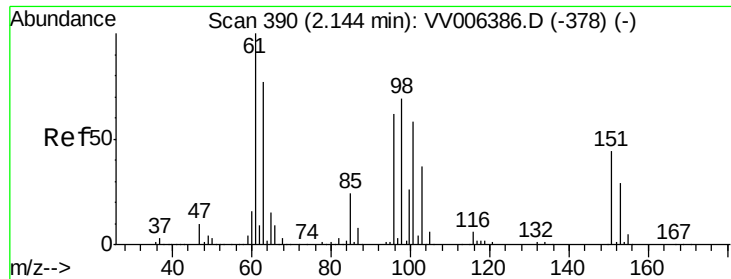

#12
 1,1-Dichloroethene
 Concen: 2.84 ug/L
 RT: 2.15 min Scan# 391
 Delta R.T. 0.00 min
 Lab File: VV006392.D
 Acq: 21 Jun 2018 14:17




Instrument :
 MSVOA_V
 ClientSampleId :
 C0KJ3


Tot Ion	Resp	Lower	Upper
96	100		
61	160.6	114.2	212.2
63	136.0	85.0	157.8

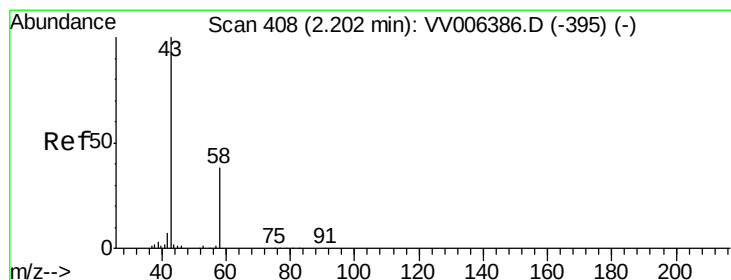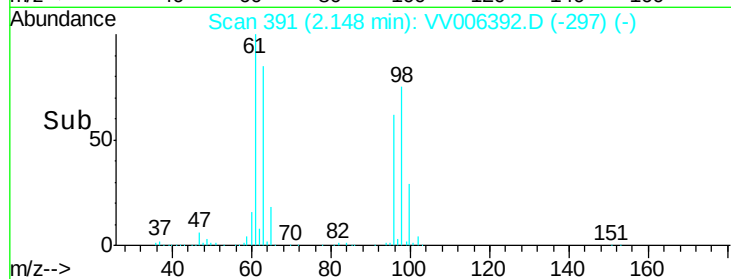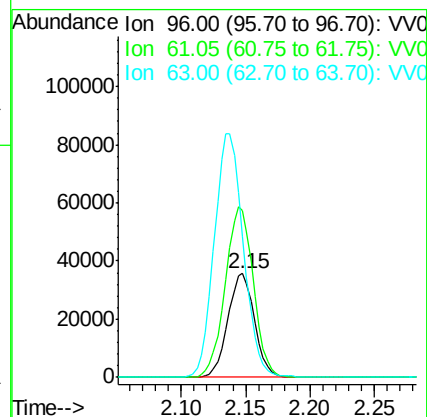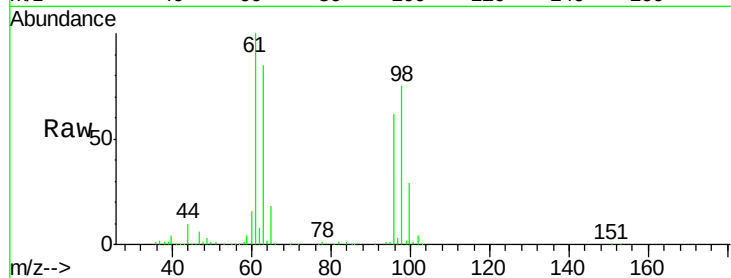

#13
 Acetone
 Concen: 8.95 ug/L
 RT: 2.21 min Scan# 411
 Delta R.T. 0.01 min
 Lab File: VV006392.D
 Acq: 21 Jun 2018 14:17

Tgt Ion	Resp	Lower	Upper
43	100		
58	39.8	0.0	67.4

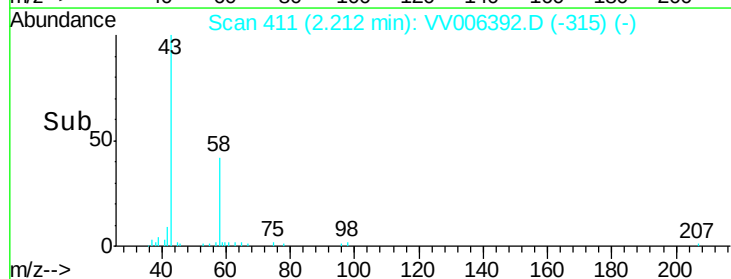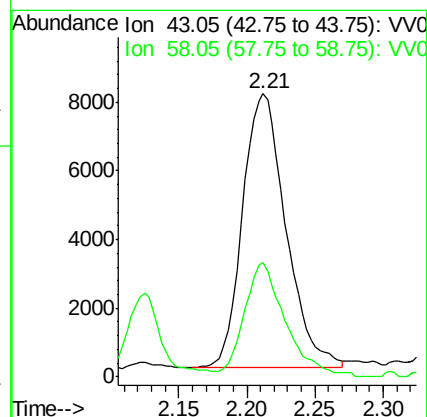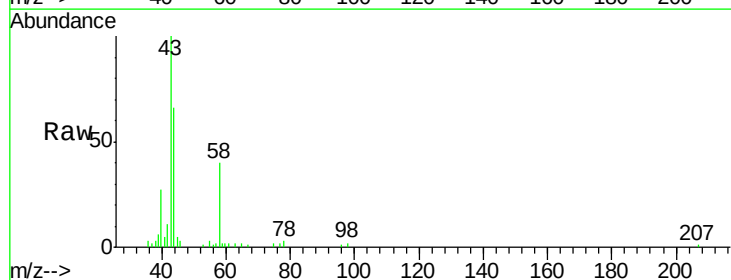

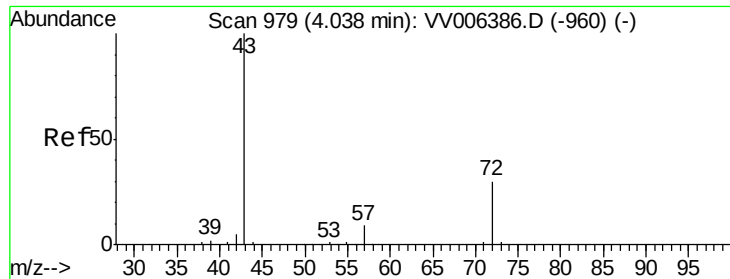

#21

2-Butanone

Concen: 4.18 ug/L

RT: 4.05 min Scan# 983

Delta R.T. 0.01 min

Lab File: VV006392.D

Acq: 21 Jun 2018 14:17

Instrument :

MSVOA_V

ClientSampleId :





C0KJ3

Tot Ion: 43 Resp: 14959

Ion Ratio Lower Upper

43 100

72 22.6 13.8 41.3

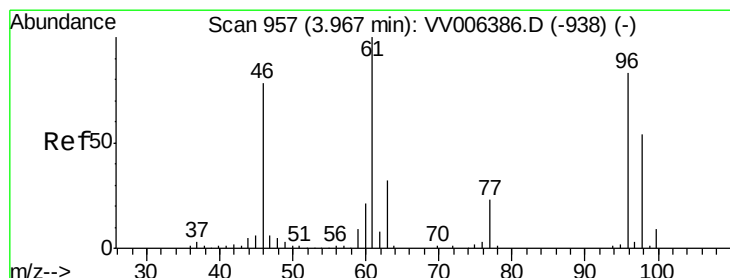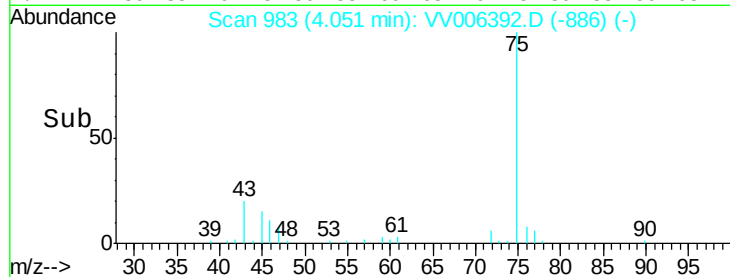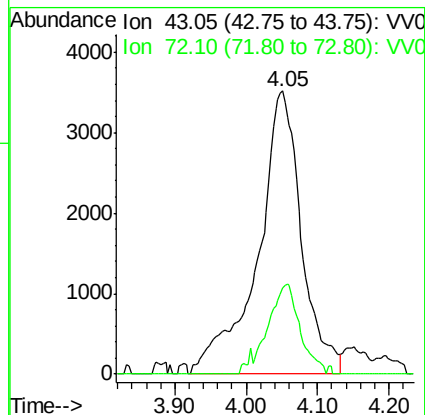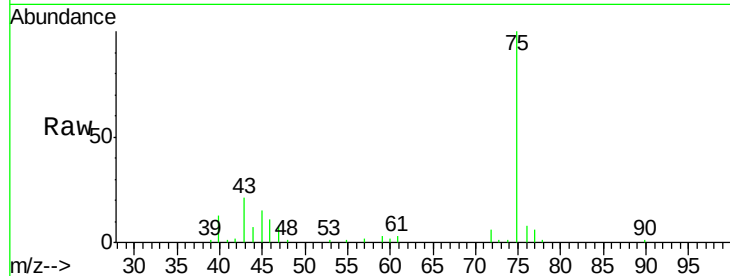

#22

cis-1,2-Dichloroethene

Concen: 0.85 ug/L

RT: 3.97 min Scan# 957

Delta R.T. 0.00 min

Lab File: VV006392.D

Acq: 21 Jun 2018 14:17




Tgt Ion: 96 Resp: 17935


Ion Ratio Lower Upper

96 100

61 112.1 84.1 156.3

68 0.0 0.3 0.5#


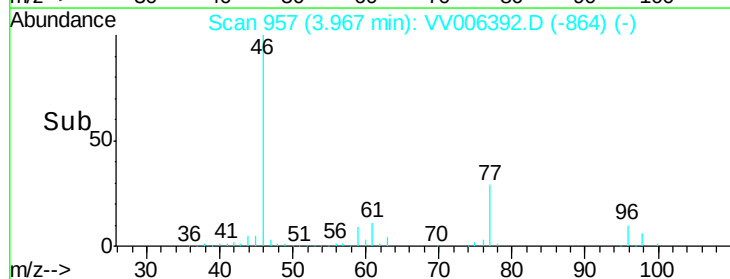
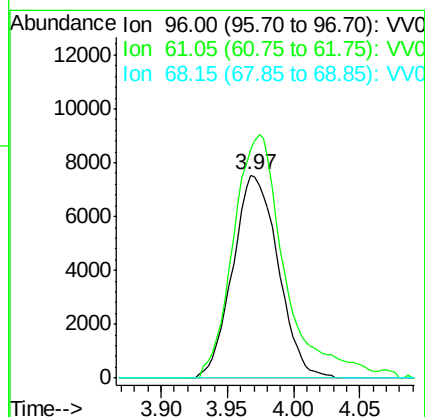
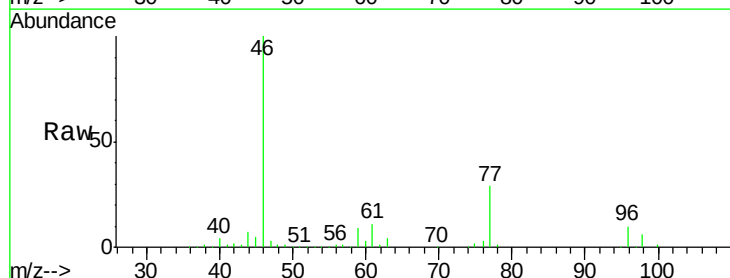


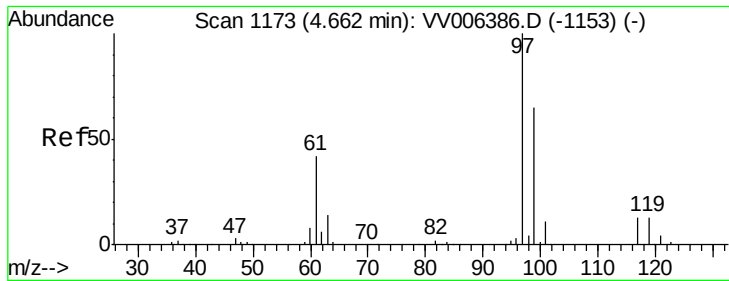

#29
 1,1,1-Trichloroethane
 Concen: 0.50 ug/L
 RT: 4.67 min Scan# 1174
 Delta R.T. 0.00 min
 Lab File: VV006392.D
 Acq: 21 Jun 2018 14:17

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KJ3

Tot Ion: 97 Resp: 15704
 Ion Ratio Lower Upper
 97 100
 99 61.4 51.5 77.3
 61 41.1 33.7 50.5

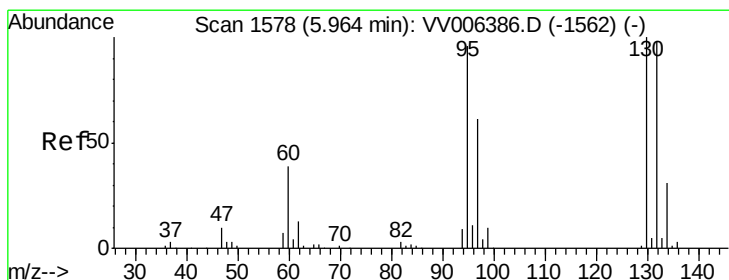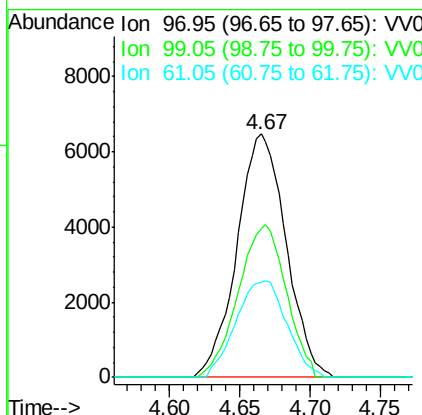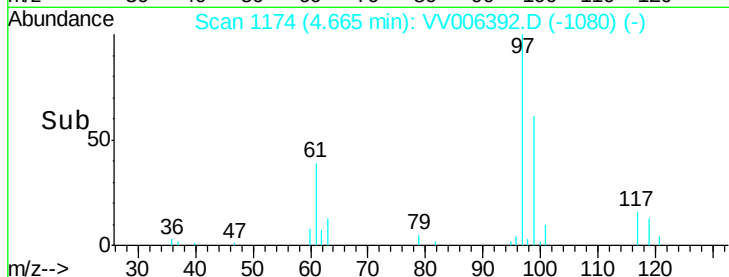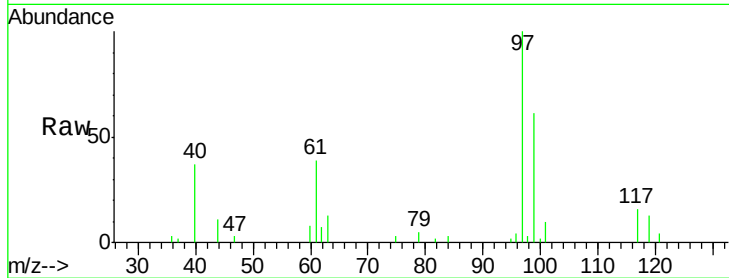

#34
 Trichloroethene
 Concen: 4.42 ug/L
 RT: 5.97 min Scan# 1579
 Delta R.T. 0.00 min
 Lab File: VV006392.D
 Acq: 21 Jun 2018 14:17

Tgt Ion: 95 Resp: 94388
 Ion Ratio Lower Upper
 95 100
 97 66.3 45.1 83.9
 132 101.8 69.0 128.1
 130 107.4 72.8 135.2

