

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062118\
 Data File : VV006393.D
 Acq On : 21 Jun 2018 15:09
 Operator : SY/MD
 Sample : J3553-14
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KK2

Quant Time: Jun 22 01:44:52 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 22 01:25:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	290160	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	263588	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	118404	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	100702	6.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	127.20%
7) Chloroethane-d5	1.58	69	80795	6.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	127.40%
11) 1,1-Dichloroethene-d2	2.13	63	137184	4.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.00%
20) 2-Butanone-d5	3.96	46	212358	63.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.22%
24) Chloroform-d	4.41	84	168451	5.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.80%
26) 1,2-Dichloroethane-d4	5.09	65	86567	5.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.80%
32) Benzene-d6	5.10	84	372702	5.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.60%
36) 1,2-Dichloropropane-d6	6.12	67	110656	5.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	116.20%
41) Toluene-d8	7.36	98	336487	5.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.40%
43) trans-1,3-Dichloropropene-	7.67	79	34113	4.00	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.00%
46) 2-Hexanone-d5	8.14	63	161687	43.95	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.90%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	64050	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	119332	5.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	8135	4.46 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062118\
Data File : VV006393.D
Acq On : 21 Jun 2018 15:09
Operator : SY/MD
Sample : J3553-14
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KK2

Quant Time: Jun 22 01:44:52 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 22 01:25:25 2018
Response via : Initial Calibration

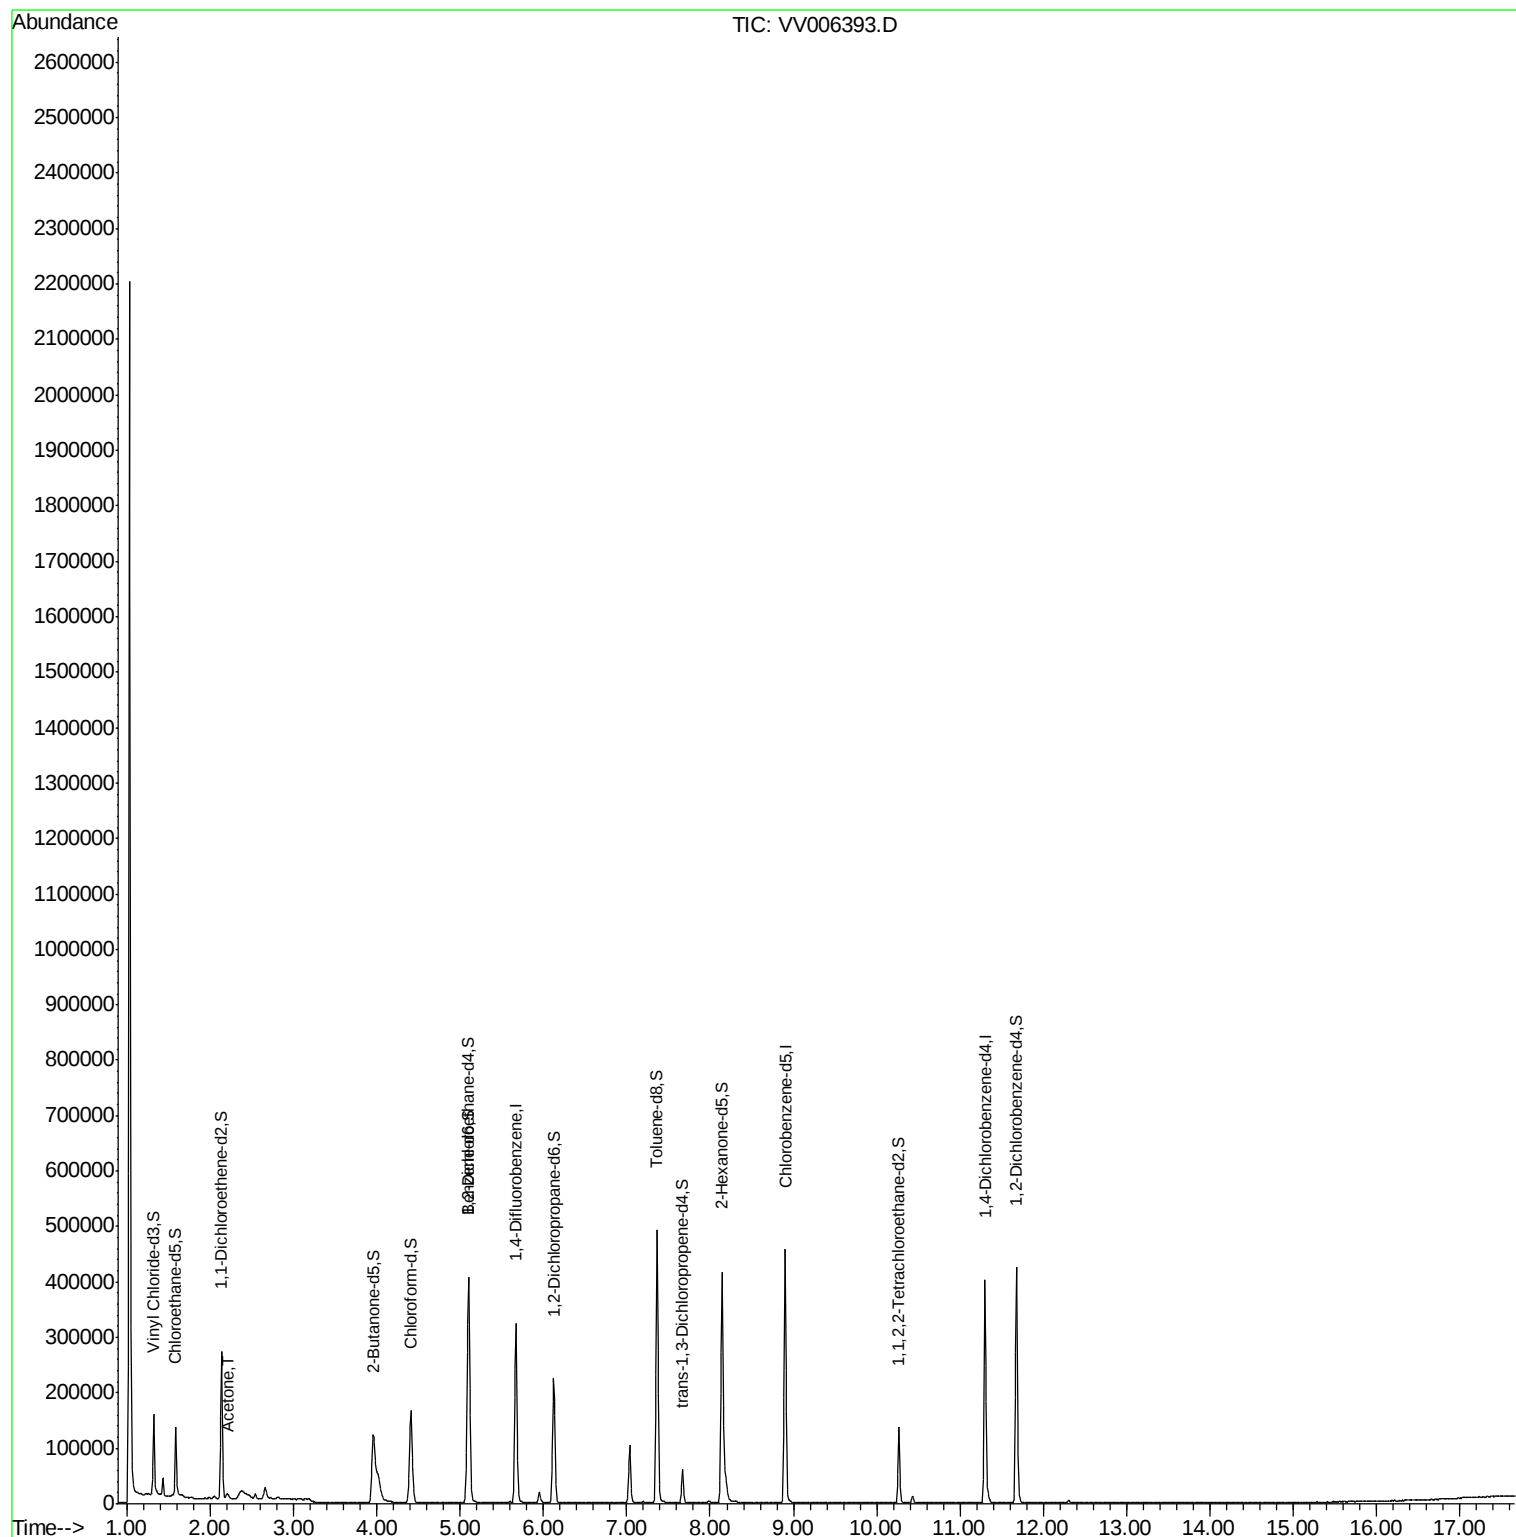

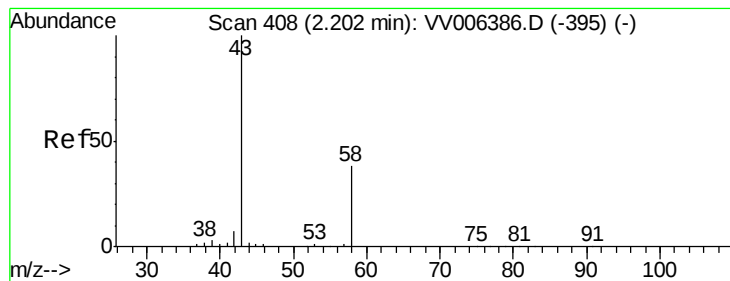

#13

Acetone

Concen: 4.46 ug/L

RT: 2.21 min Scan# 411

Delta R.T. 0.01 min

Lab File: VV006393.D

Acq: 21 Jun 2018 15:09

Instrument :
MSVOA_V
ClientSampleId :
C0KK2

Tot Ion: 43 Resp: 8135

Ion Ratio Lower Upper

43 100

58 36.6 0.0 67.4

