

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062119\
 Data File : VV011649.D
 Acq On : 20 Jun 2019 18:19
 Operator : SY/MD
 Sample : K3381-19
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCT0

Quant Time: Jun 21 02:53:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 21 02:33:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	156402	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	142591	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	59190	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	49878	4.80	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.00%
7) Chloroethane-d5	1.56	69	37386	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.40%
11) 1,1-Dichloroethene-d2	2.12	63	76541	3.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.60%
20) 2-Butanone-d5	3.94	46	157633	57.65	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.30%
24) Chloroform-d	4.40	84	91192	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
26) 1,2-Dichloroethane-d4	5.08	65	59748	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.00%
32) Benzene-d6	5.09	84	204382	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.80%
36) 1,2-Dichloropropane-d6	6.12	67	63400	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.36	98	173915	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
43) trans-1,3-Dichloropropene-	7.67	79	19642	4.59	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.80%
46) 2-Hexanone-d5	8.14	63	118338	58.91	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	117.82%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	45520	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	58499	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	4472	2.264 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062119\
Data File : VV011649.D
Acq On : 20 Jun 2019 18:19
Operator : SY/MD
Sample : K3381-19
Misc : 25ML/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCT0

Quant Time: Jun 21 02:53:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 21 02:33:37 2019
Response via : Initial Calibration

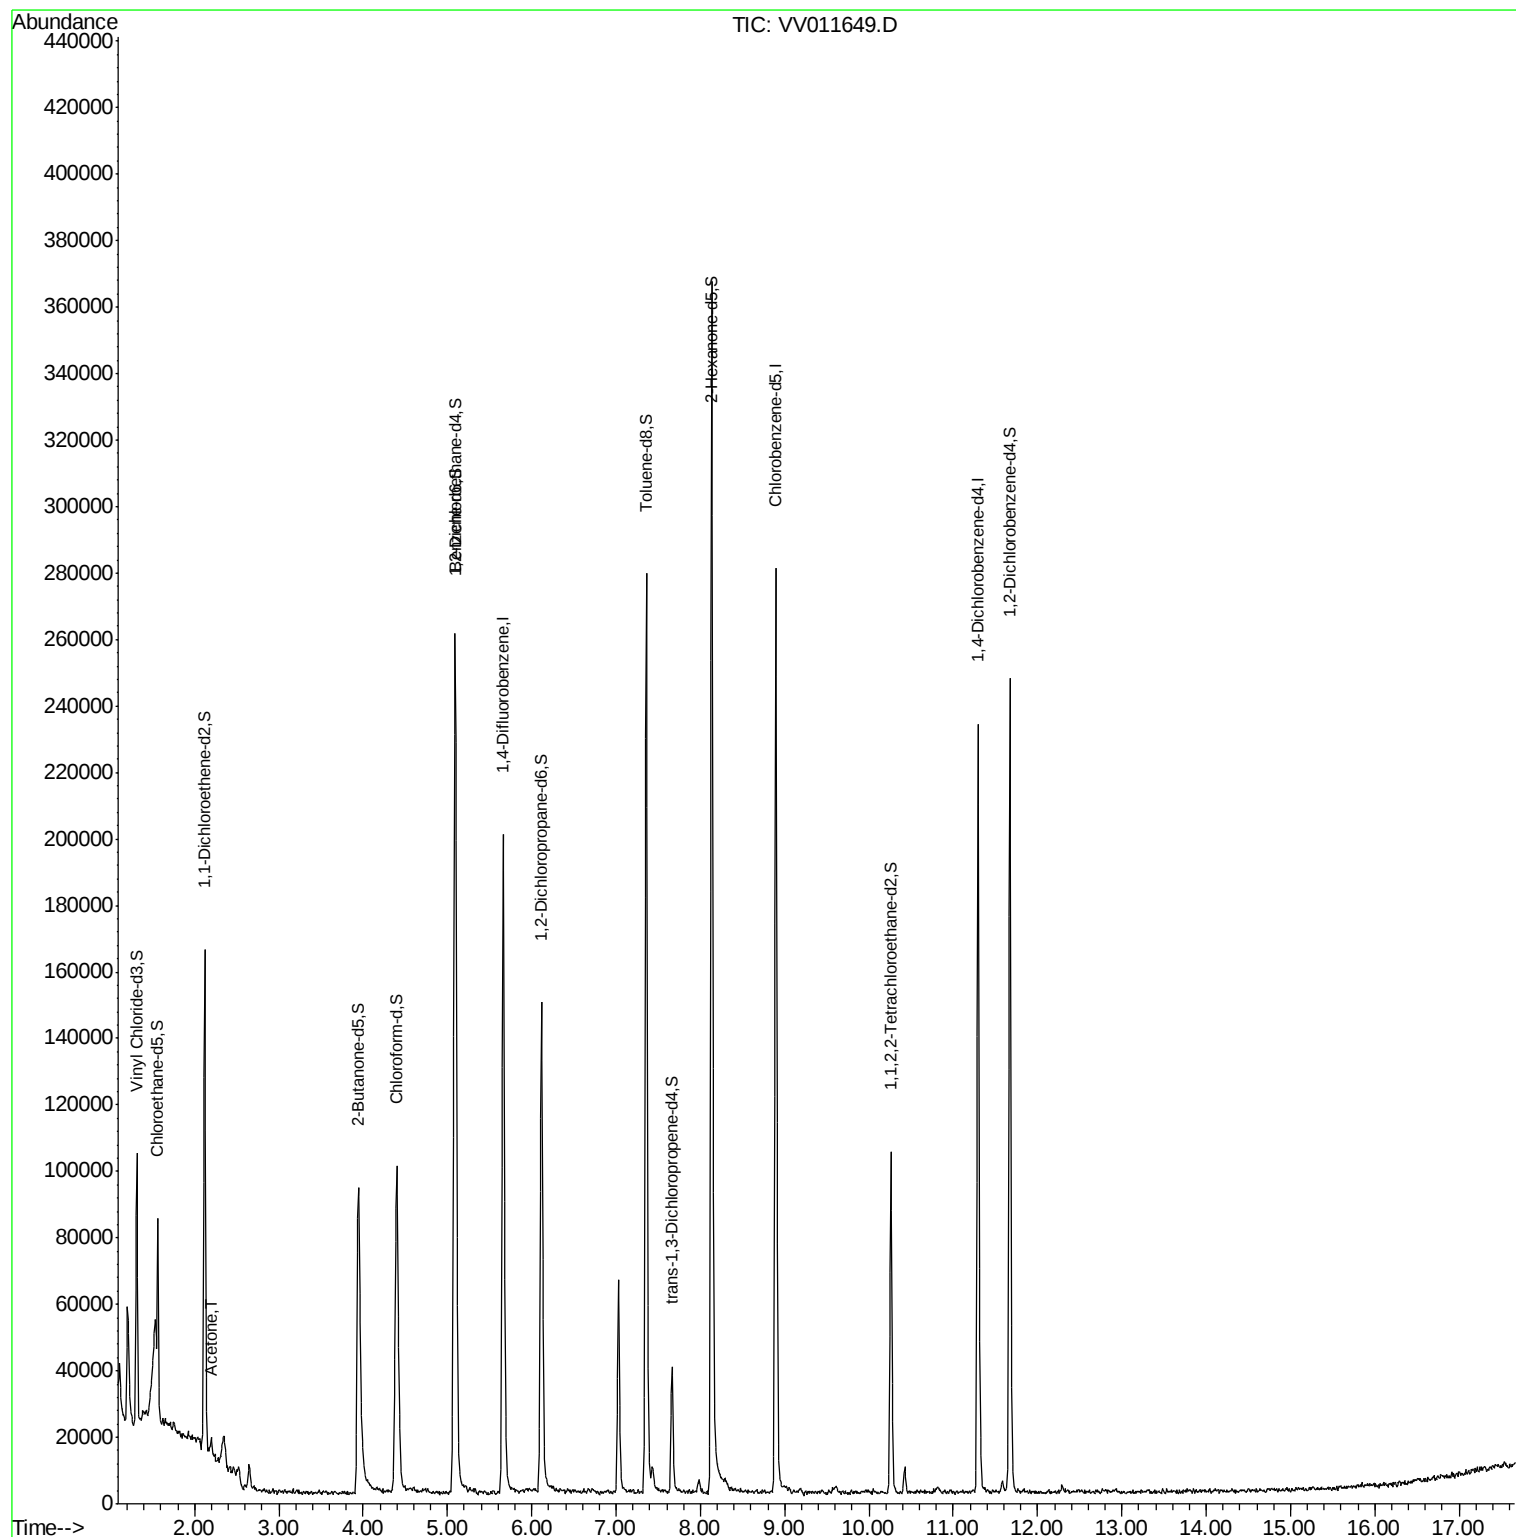

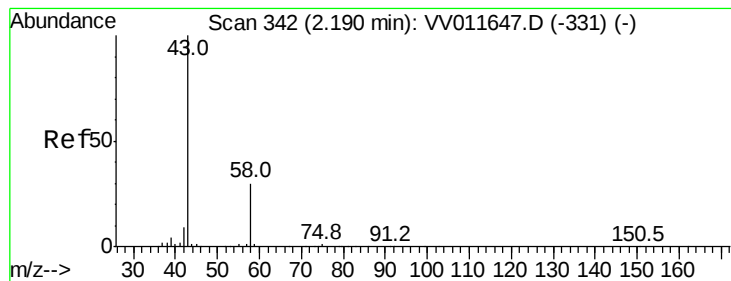

#13

Acetone

Concen: 2.264 ug/L

RT: 2.20 min Scan# 344

Delta R.T. 0.01 min

Lab File: VV011649.D

Acq: 20 Jun 2019 18:19

Instrument :
MSVOA_V
ClientSampleId :
BFCT0

Tot Ion: 43 Resp: 4472

Ion Ratio Lower Upper

43 100

58 26.4 0.0 56.6

