


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062119\
Data File : VV011633.D
Acq On : 20 Jun 2019 08:51
Operator : SY/MD
Sample : BFB53
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB53

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jun 21 04:33:10 2019

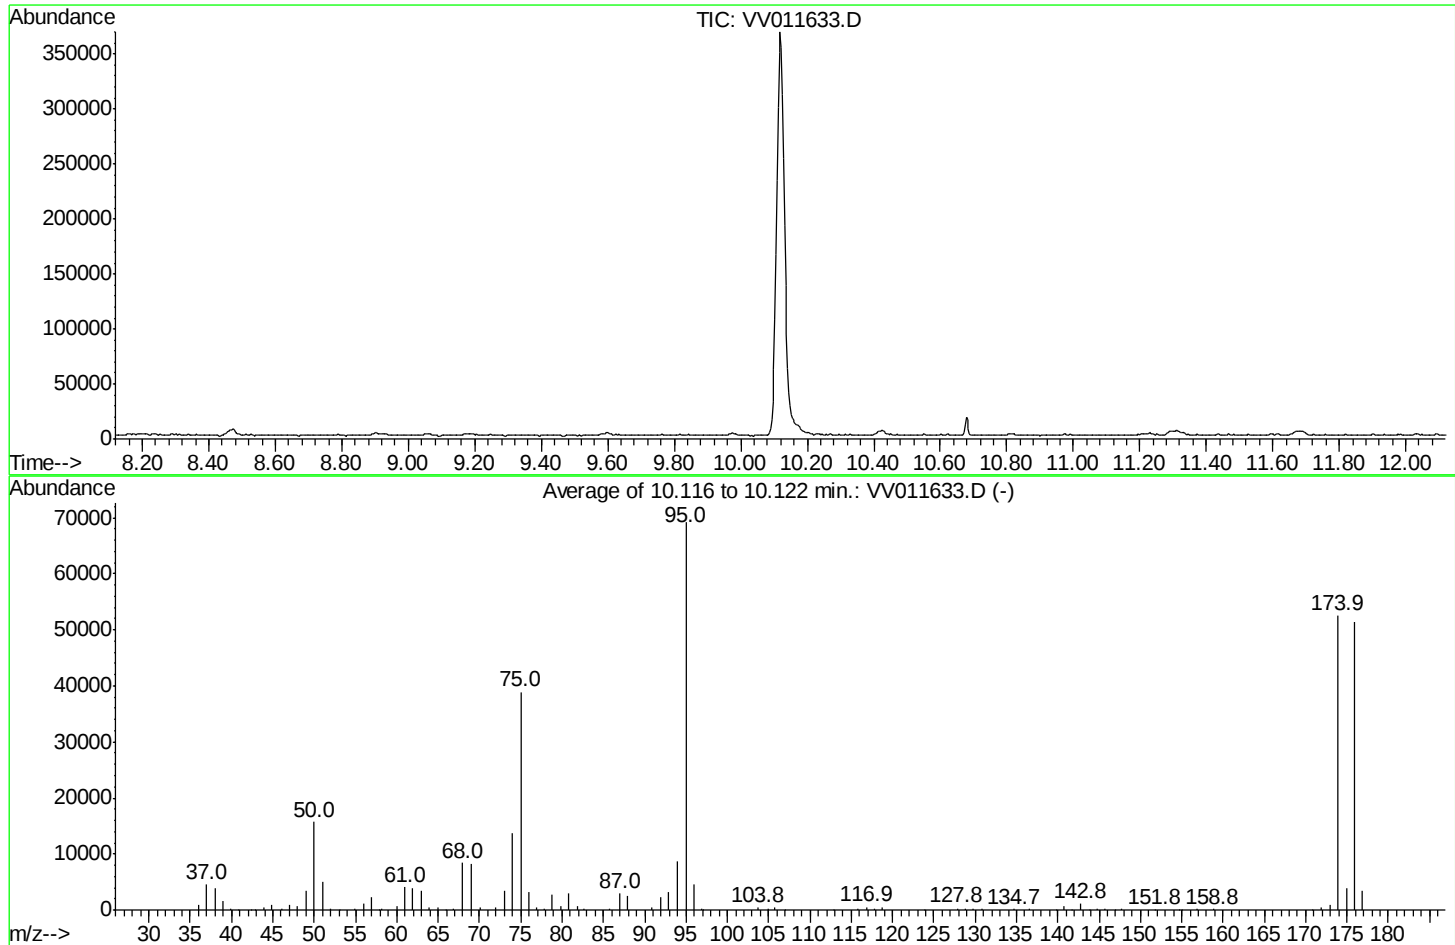

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	15660	PASS
75	95	30	80	56.3	38928	PASS
95	95	100	100	100.0	69202	PASS
96	95	5	9	6.6	4541	PASS
173	174	0.00	2	1.8	933	PASS
174	95	50	120	75.8	52482	PASS
175	174	5	9	7.5	3947	PASS
176	174	95	101	98.1	51496	PASS
177	176	5	9	6.7	3458	PASS

Scan 2794 (10.074 min): VV011633.D
BFB53

m/z	Abundance
35.60	106.0
37.40	124.0
39.90	2078.0
41.90	128.0
42.90	111.0
43.80	360.0
45.80	114.0
54.50	119.0
66.70	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
35.90	985.0
37.00	4486.0
38.00	4066.0
39.00	1603.0
39.90	2393.0
40.80	115.0
42.90	125.0
43.90	863.0
44.90	851.0
46.00	160.0
47.00	983.0
47.90	672.0
49.00	3460.0
50.00	15486.0
51.00	5102.0
51.90	285.0
53.00	102.0
55.00	294.0
56.00	1173.0
57.00	2354.0
58.10	156.0
60.00	749.0
61.00	4187.0
61.90	4133.0
63.00	3251.0
63.90	467.0
64.90	382.0
66.90	267.0
68.00	8296.0
69.00	8078.0
70.10	604.0
72.00	498.0
73.00	3488.0
74.00	13773.0
75.00	38736.0
76.00	3122.0
76.90	559.0
77.90	380.0
78.80	2665.0
79.90	802.0
80.90	2905.0
81.90	669.0
82.70	143.0
85.80	121.0
87.00	2668.0
87.90	2666.0
90.80	404.0
91.90	2082.0
92.90	3218.0
94.00	8473.0
95.00	67880.0
96.00	4288.0
96.90	302.0
103.70	424.0
104.90	189.0
105.70	386.0
115.90	293.0
116.90	524.0
117.80	270.0
118.80	371.0
123.80	103.0
127.90	311.0
128.80	165.0
129.80	281.0
130.90	128.0
134.70	190.0
136.60	186.0
139.80	114.0
140.80	777.0
142.80	988.0
144.00	126.0
144.80	215.0
145.70	162.0
147.70	179.0
154.70	156.0
156.80	182.0
158.90	173.0
170.80	107.0
171.90	368.0
172.90	915.0
173.90	49928.0
174.90	3576.0
175.90	49648.0
176.90	3615.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
36.00	1015.0
37.00	4775.0
38.00	4014.0
39.00	1677.0
39.90	2424.0
40.80	124.0
41.80	102.0
42.90	137.0
43.90	927.0
44.90	876.0
46.10	170.0
47.00	979.0
47.90	758.0
49.00	3476.0
50.00	16129.0
51.00	5322.0
51.90	257.0
55.00	300.0
56.00	1209.0
57.00	2274.0
58.20	146.0
60.00	778.0
61.00	4248.0
61.90	4066.0
63.00	3553.0
63.90	459.0
64.90	408.0
65.90	111.0
66.80	269.0
68.00	8679.0
69.00	8386.0
70.10	564.0
71.90	542.0
73.00	3542.0
74.00	14185.0
75.00	40024.0
76.00	3328.0
77.00	560.0
77.90	366.0
78.80	2858.0
79.90	803.0
80.80	3018.0
81.90	733.0
82.70	185.0
85.80	131.0
87.00	3028.0
87.90	2701.0
90.80	441.0
92.00	2226.0
92.90	3413.0
94.00	8982.0
95.00	71288.0
96.00	4692.0
96.90	259.0
103.80	454.0
104.90	253.0
105.80	425.0
106.90	148.0
112.90	107.0
115.80	316.0
116.90	604.0
117.80	290.0
118.70	387.0
127.90	304.0
128.80	176.0
129.80	282.0
130.80	140.0
134.70	213.0
136.60	194.0
140.80	763.0
141.70	111.0
142.80	1094.0
143.90	120.0
144.80	236.0
145.80	206.0
146.90	108.0
147.70	173.0
151.80	133.0
154.70	111.0
156.90	157.0
158.90	197.0
170.90	127.0
171.80	419.0
172.90	982.0
173.90	54160.0
174.90	4053.0
175.90	53160.0
176.90	3582.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
36.00	931.0
37.00	4369.0
38.00	3621.0
39.00	1597.0
39.90	2417.0
40.80	110.0
41.80	130.0
42.30	108.0
42.90	135.0
43.90	932.0
44.90	785.0
45.90	151.0
46.10	149.0
47.00	844.0
47.90	757.0
48.90	3275.0
50.00	15366.0
51.00	4876.0
51.90	205.0
54.90	302.0
56.00	1203.0
56.90	2099.0
57.80	125.0
58.30	130.0
60.00	759.0
61.00	3779.0
61.90	3613.0
63.00	3365.0
63.90	422.0
65.00	354.0
65.90	125.0
66.80	260.0
68.00	8101.0
69.00	8070.0
70.10	516.0
71.90	571.0
73.00	3496.0
74.00	13457.0
75.00	38024.0
76.00	3157.0
77.00	529.0
77.90	307.0
78.80	2842.0
79.90	776.0
80.80	2859.0
81.90	741.0
82.70	183.0
85.80	121.0
87.00	3108.0
87.90	2484.0
90.80	443.0
92.00	2246.0
92.90	3296.0
94.00	8682.0
95.00	68440.0
96.00	4643.0
97.10	172.0
103.80	423.0
104.90	264.0
105.80	406.0
106.90	177.0
112.90	133.0
115.70	296.0
116.90	582.0
117.80	302.0
118.70	405.0
127.80	257.0
128.80	165.0
129.80	238.0
130.80	136.0
134.70	205.0
136.60	172.0
140.80	815.0
141.70	109.0
142.80	1048.0
143.80	105.0
144.80	212.0
145.80	186.0
146.90	131.0
147.70	156.0
151.80	140.0
155.00	137.0
156.90	122.0
158.80	149.0
171.80	476.0
173.00	903.0
173.90	53360.0
174.90	4212.0
175.90	51680.0
176.90	3177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53