




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026481.D
 Acq On : 21 Jun 2022 12:21
 Operator : SY/MD
 Sample : N3358-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T4

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:41:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

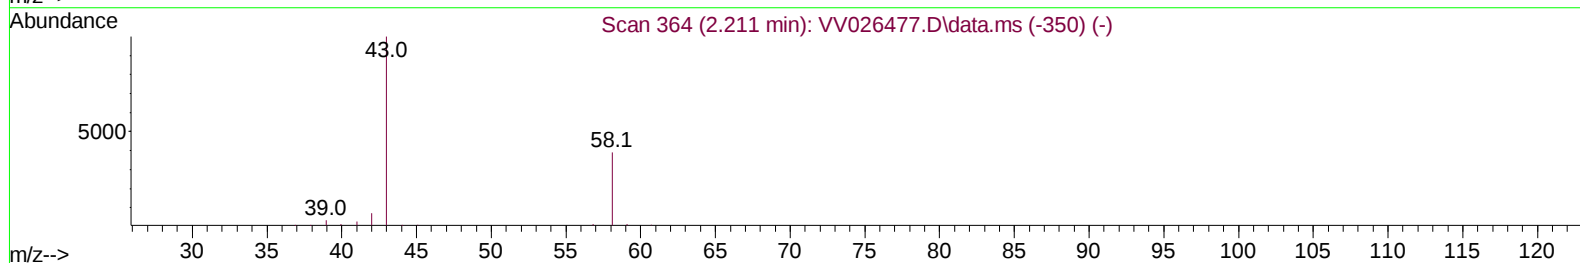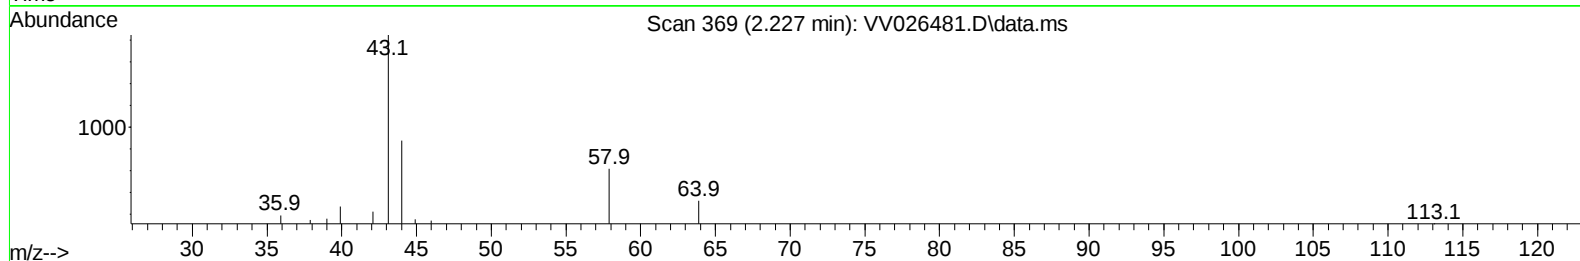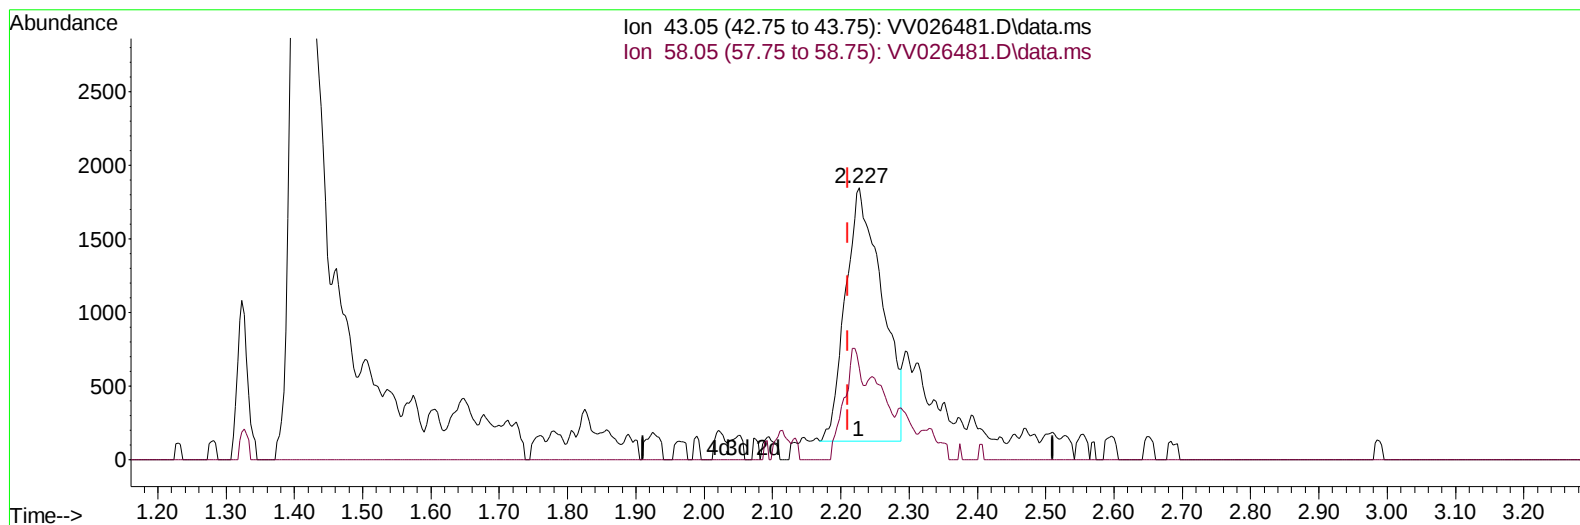

TIC: VV026481.D\data.ms

(13) Acetone (T)

2.227min (+ 0.016) 5.23 ug/L

response 6365

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	21.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026481.D
Acq On : 21 Jun 2022 12:21
Operator : SY/MD
Sample : N3358-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4T4

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:41:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

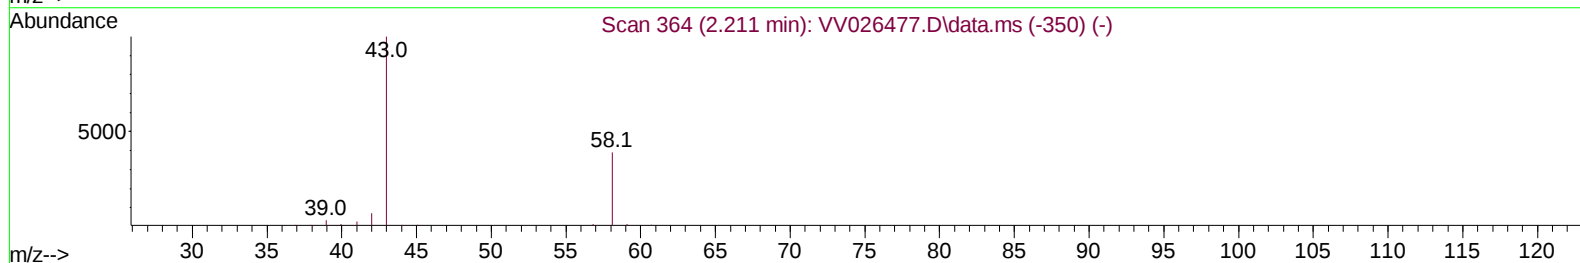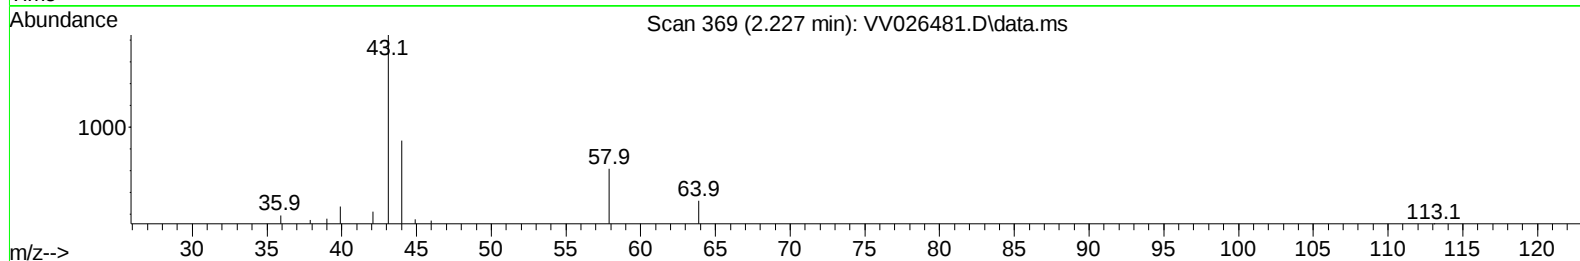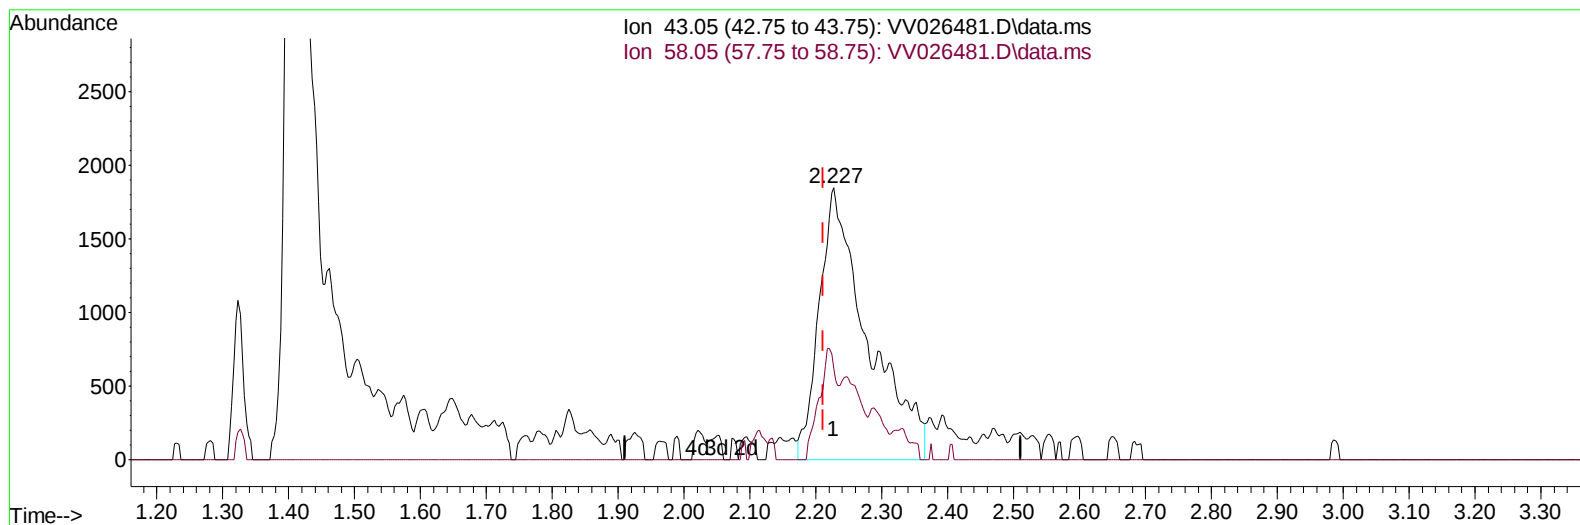

TIC: VV026481.D\data.ms

(13) Acetone (T)

2.227min (+ 0.016) 7.73 ug/L m

response 9405

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	14.32
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026481.D
 Acq On : 21 Jun 2022 12:21
 Operator : SY/MD
 Sample : N3358-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T4

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:41:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	185214	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	174513	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73257	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	63508	3.948	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	79.000%	
7) Chloroethane-d5	1.584	69	57187	4.521	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	90.400%	
11) 1,1-Dichloroethene-d2	2.124	63	94596	3.424	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	68.400%	
20) 2-Butanone-d5	3.934	46	81921	52.188	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	104.380%	
24) Chloroform-d	4.365	84	127611	5.412	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	108.200%	
26) 1,2-Dichloroethane-d4	5.047	65	51732	5.186	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	103.800%	
32) Benzene-d6	5.063	84	244711	5.245	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	104.800%	
36) 1,2-Dichloropropane-d6	6.076	67	72676	5.337	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	106.800%	
41) Toluene-d8	7.320	98	199767	4.696	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	94.000%	
43) trans-1,3-Dichloroprop...	7.632	79	17221	3.900	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	78.000%	
46) 2-Hexanone-d5	8.095	63	65650	49.220	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	98.440%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	46555	5.550	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	111.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	63901	5.663	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	113.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.227	43	9405m	7.731	ug/L	
25) Chloroform	4.387	83	9280	0.395	ug/L	100
38) Bromodichloromethane	6.526	83	3431	0.242	ug/L	96
42) Toluene	7.397	91	21400	0.455	ug/L	98
52) Ethylbenzene	9.021	91	2010	0.043	ug/L #	79
53) m,p-Xylene	9.143	106	3757	0.204	ug/L	82
54) o-Xylene	9.548	106	1236	0.069	ug/L	97
63) 1,2,4-Trimethylbenzene	10.924	105	3016	0.098	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026481.D
Acq On : 21 Jun 2022 12:21
Operator : SY/MD
Sample : N3358-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4T4

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:41:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

