




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026482.D
Acq On : 21 Jun 2022 12:44
Operator : SY/MD
Sample : N3345-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK8

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:41:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

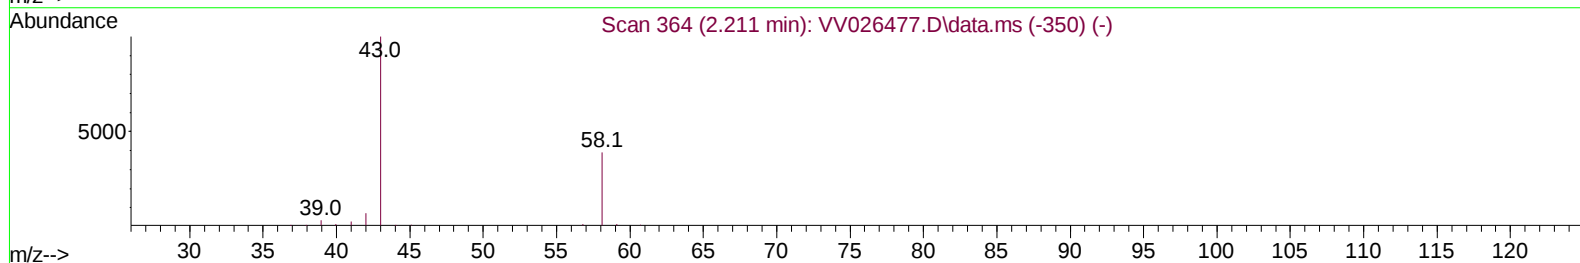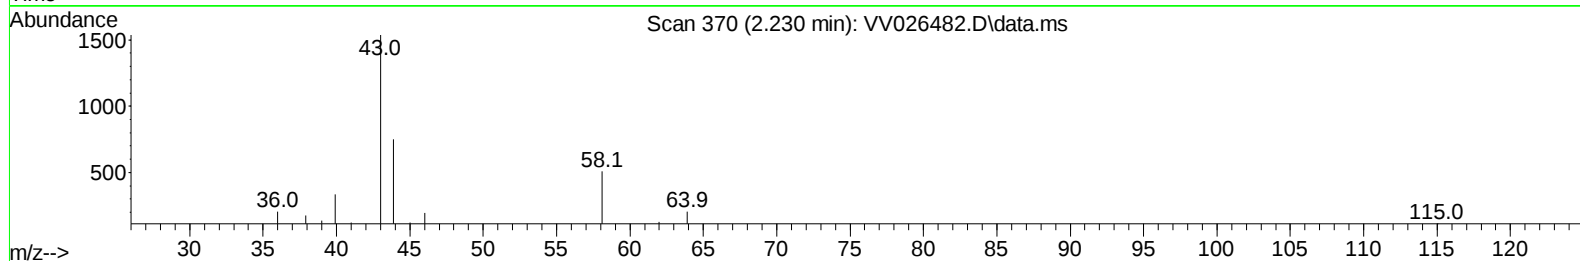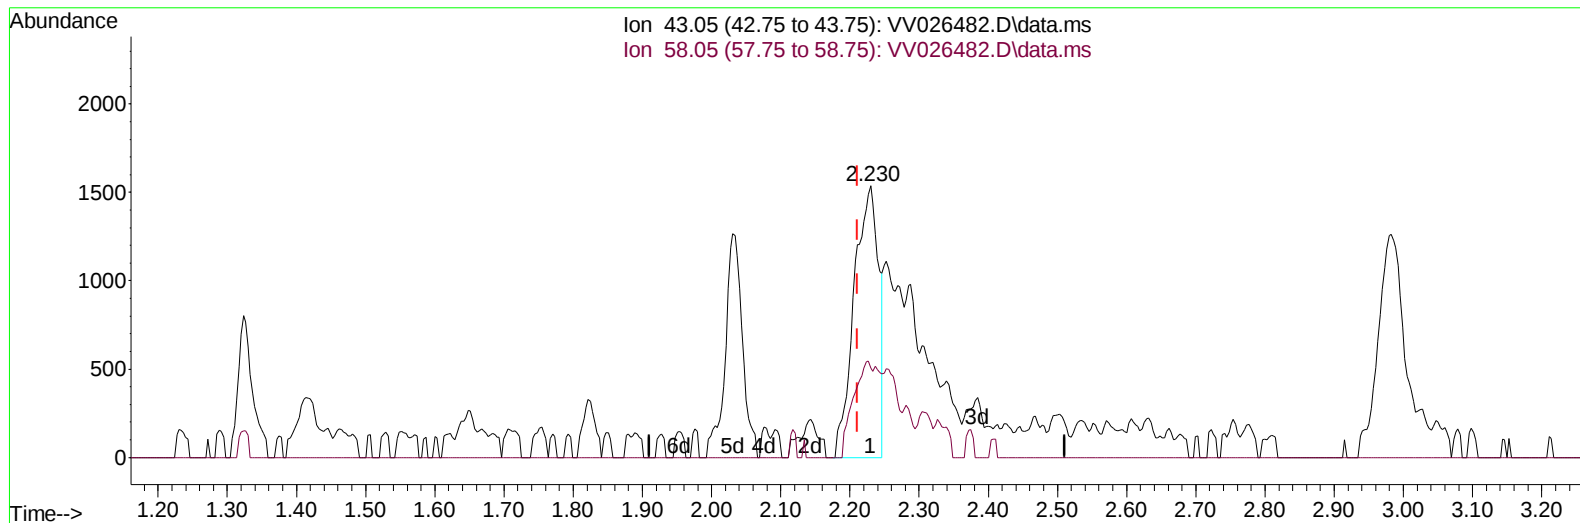

TIC: VV026482.D\data.ms

(13) Acetone (T)

2.230min (+ 0.019) 3.23 ug/L

response 3794

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	27.81
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026482.D
 Acq On : 21 Jun 2022 12:44
 Operator : SY/MD
 Sample : N3345-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:41:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

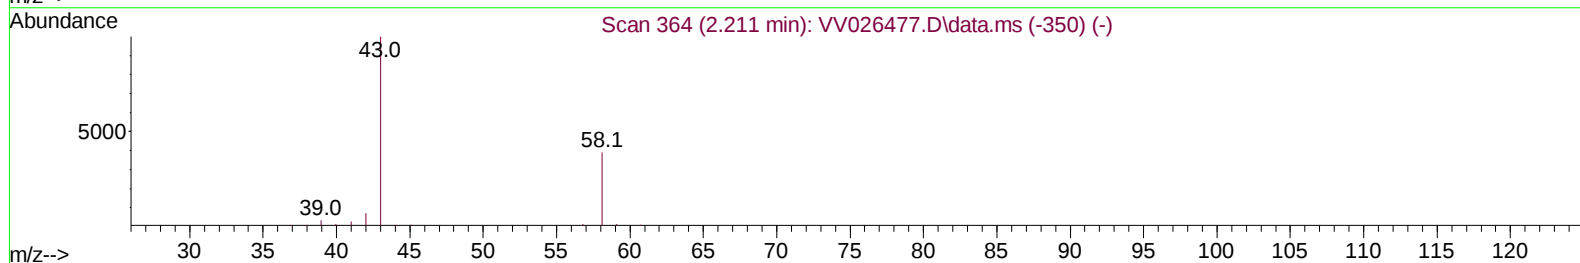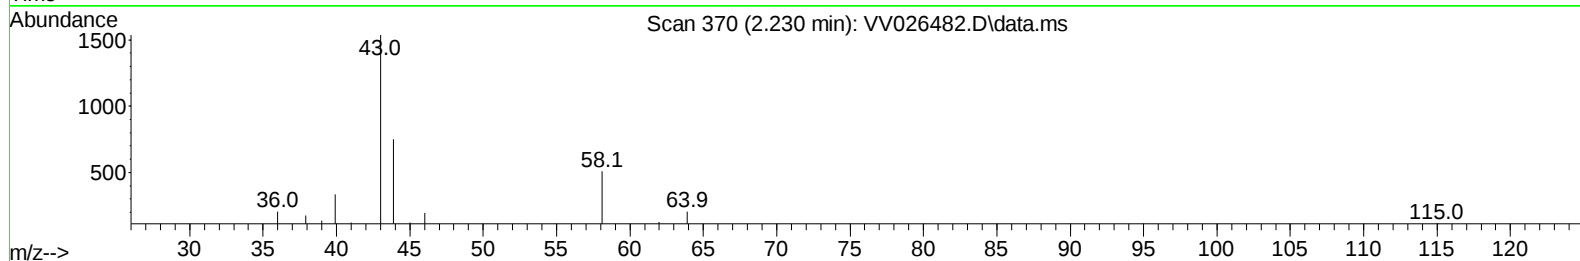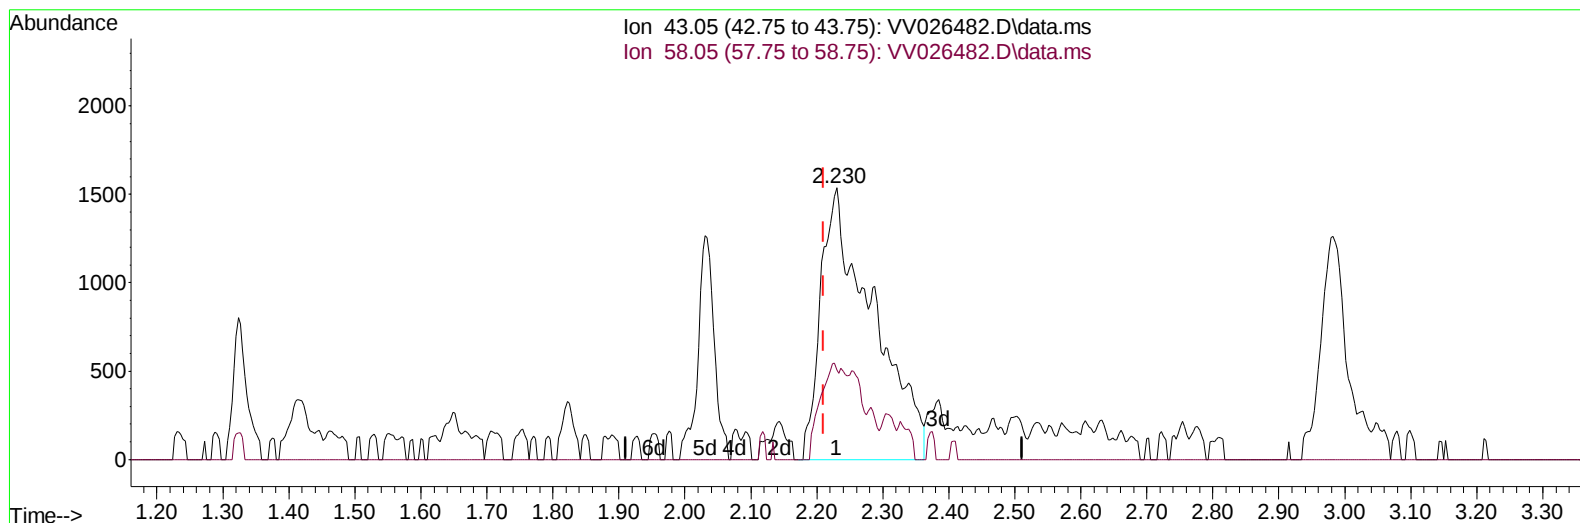

TIC: VV026482.D\data.ms

(13) Acetone (T)

2.230min (+ 0.019) 7.10 ug/L m

response 8331

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	12.66
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026482.D
 Acq On : 21 Jun 2022 12:44
 Operator : SY/MD
 Sample : N3345-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:41:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	178614	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	172778	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70786	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	62593	4.035	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	80.600%	
7) Chloroethane-d5	1.584	69	54651	4.480	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	89.600%	
11) 1,1-Dichloroethene-d2	2.124	63	94551	3.549	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	71.000%	
20) 2-Butanone-d5	3.937	46	80443	53.140	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	106.280%	
24) Chloroform-d	4.365	84	128494	5.651	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	113.000%	
26) 1,2-Dichloroethane-d4	5.047	65	50257	5.224	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	104.400%	
32) Benzene-d6	5.063	84	238969	5.173	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.400%	
36) 1,2-Dichloropropane-d6	6.076	67	74058	5.493	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	109.800%	
41) Toluene-d8	7.320	98	208945	4.961	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.200%	
43) trans-1,3-Dichloroprop...	7.629	79	16621	3.802	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	76.000%	
46) 2-Hexanone-d5	8.095	63	65948	49.940	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	99.880%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44701	5.382	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	107.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	62526	5.735	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	114.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.230	43	8331m	7.101	ug/L	
14) Carbon disulfide	2.311	76	8494	0.305	ug/L	100
25) Chloroform	4.391	83	53847	2.378	ug/L	99
42) Toluene	7.404	91	10899	0.234	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026482.D
Acq On : 21 Jun 2022 12:44
Operator : SY/MD
Sample : N3345-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:41:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

