




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026483.D
 Acq On : 21 Jun 2022 13:08
 Operator : SY/MD
 Sample : N3345-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK9

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:42:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

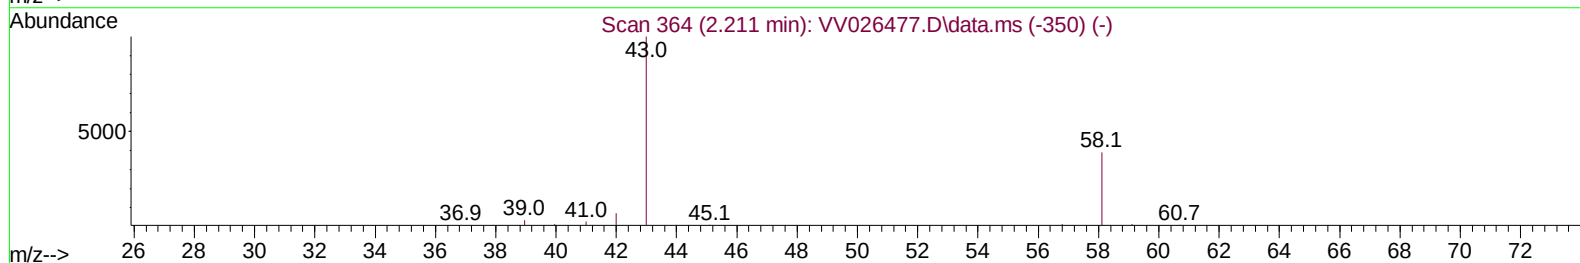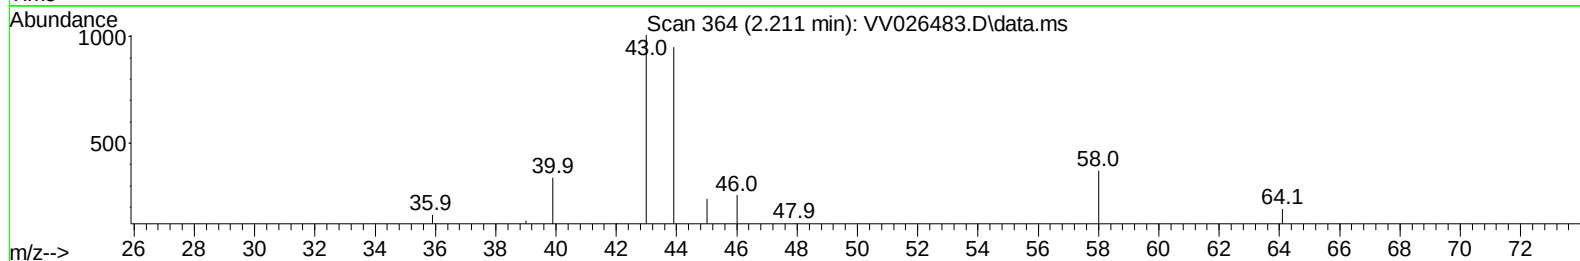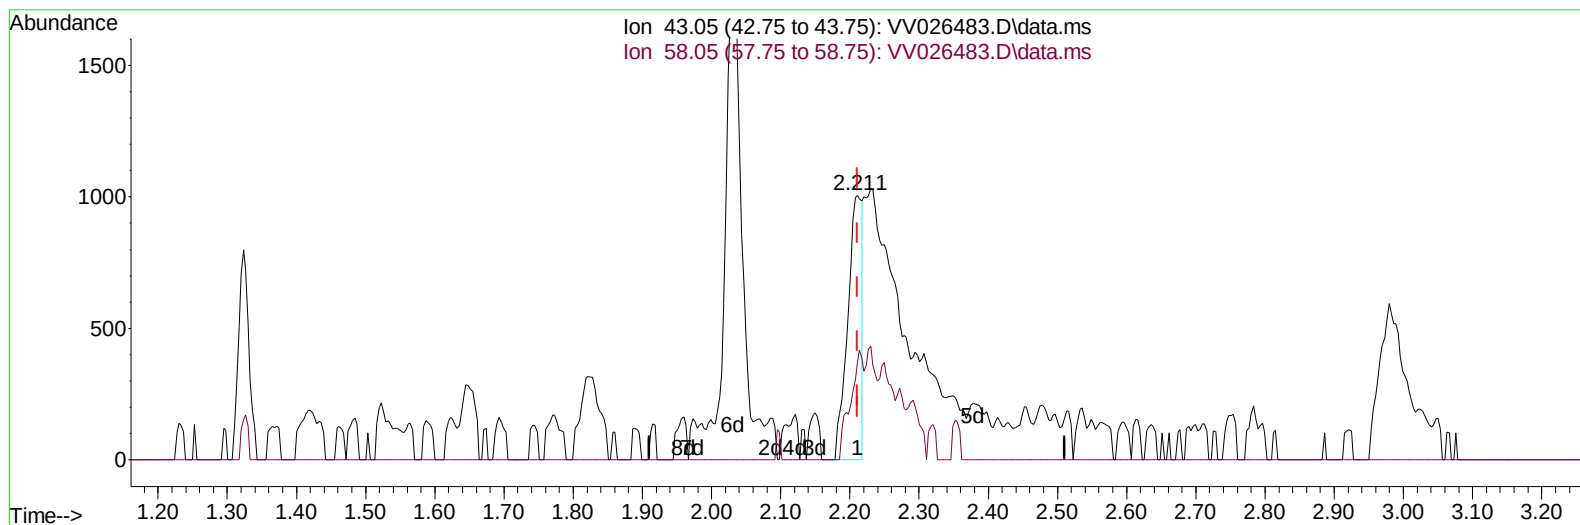

TIC: VV026483.D\data.ms

(13) Acetone (T)

2.211min (+ 0.000) 1.22 ug/L

response 1453

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	38.89
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026483.D
 Acq On : 21 Jun 2022 13:08
 Operator : SY/MD
 Sample : N3345-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK9

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:42:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

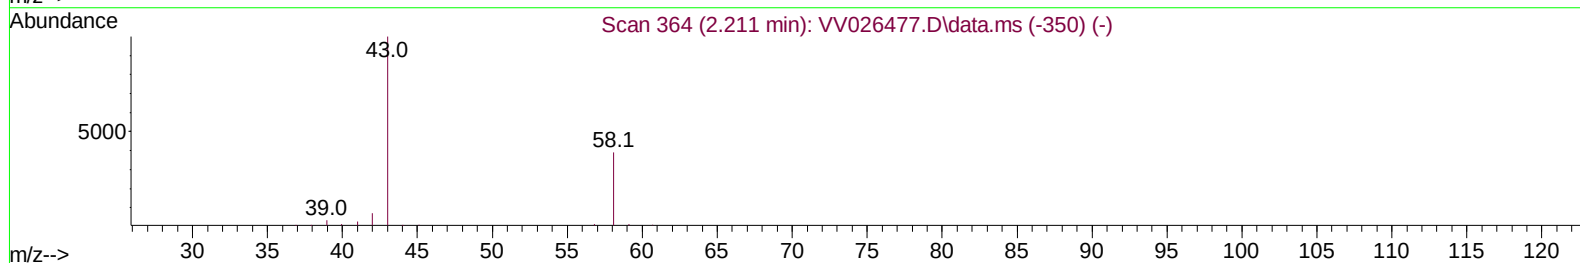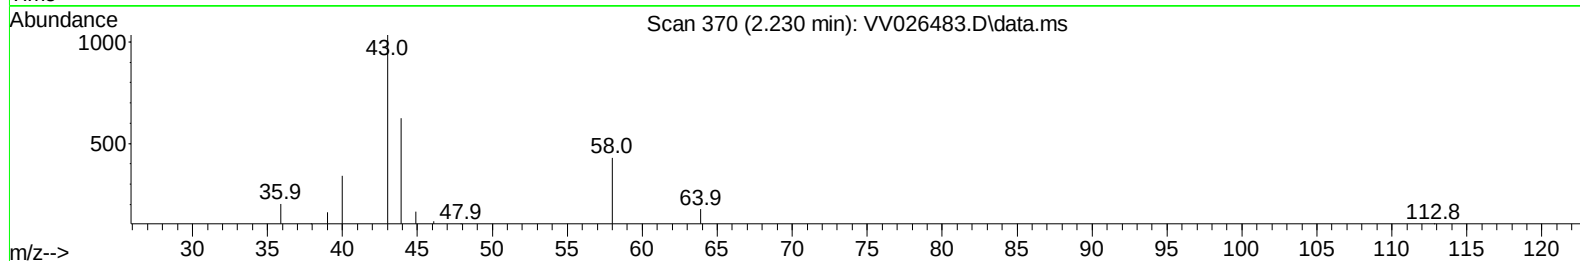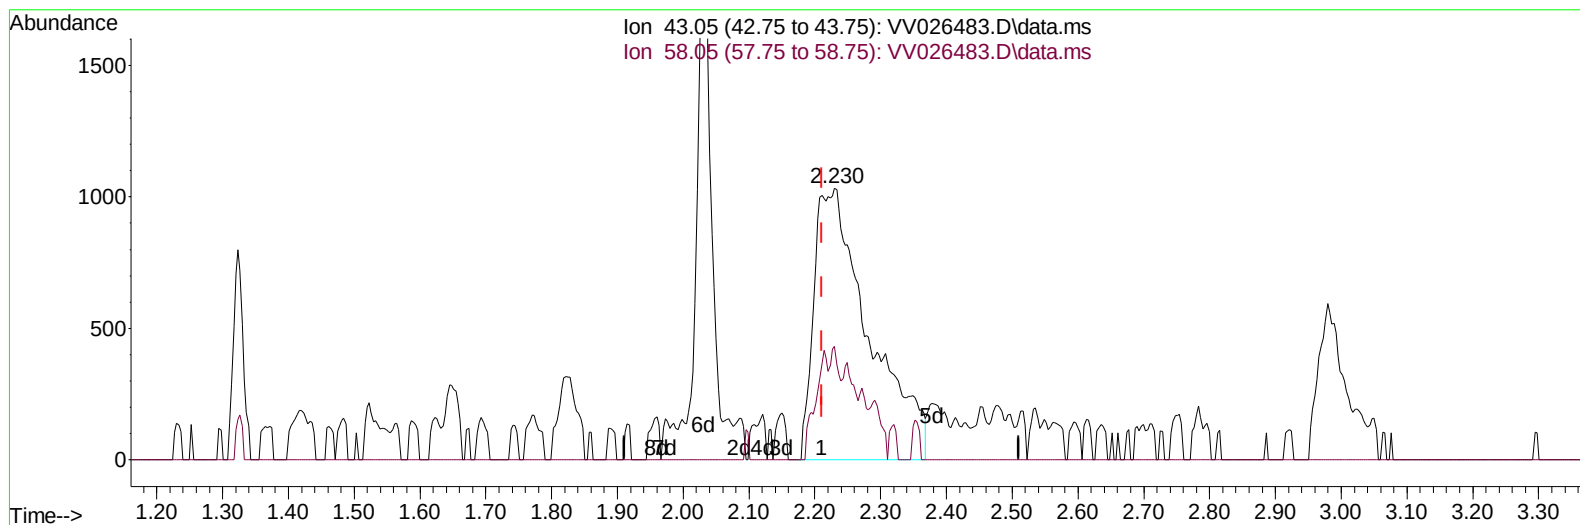

TIC: VV026483.D\data.ms

(13) Acetone (T)

2.230min (+ 0.019) 5.04 ug/L m

response 5994

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	9.43
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026483.D
 Acq On : 21 Jun 2022 13:08
 Operator : SY/MD
 Sample : N3345-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK9

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:42:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	180945	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	172111	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72233	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	64196	4.085	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	81.600%		
7) Chloroethane-d5	1.584	69	55638	4.502	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	90.000%		
11) 1,1-Dichloroethene-d2	2.124	63	93562	3.467	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	69.400%		
20) 2-Butanone-d5	3.934	46	84448	55.067	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	110.140%		
24) Chloroform-d	4.362	84	129764	5.633	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	112.600%		
26) 1,2-Dichloroethane-d4	5.047	65	52179	5.354	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	107.000%		
32) Benzene-d6	5.063	84	244546	5.315	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	106.200%		
36) 1,2-Dichloropropane-d6	6.076	67	72842	5.424	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	108.400%		
41) Toluene-d8	7.320	98	203137	4.842	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	96.800%		
43) trans-1,3-Dichloroprop...	7.632	79	17738	4.073	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	81.400%		
46) 2-Hexanone-d5	8.095	63	67344	51.195	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	102.380%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46989	5.680	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	113.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152	63464	5.704	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	114.000%		
Target Compounds						
					Qvalue	
13) Acetone	2.230	43	5994m	5.044	ug/L	
14) Carbon disulfide	2.311	76	8836	0.313	ug/L	97
25) Chloroform	4.391	83	56017	2.442	ug/L	97
42) Toluene	7.400	91	9943	0.214	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026483.D
Acq On : 21 Jun 2022 13:08
Operator : SY/MD
Sample : N3345-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK9

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:42:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

