




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026488.D
 Acq On : 21 Jun 2022 15:06
 Operator : SY/MD
 Sample : N3355-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C4

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:43:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

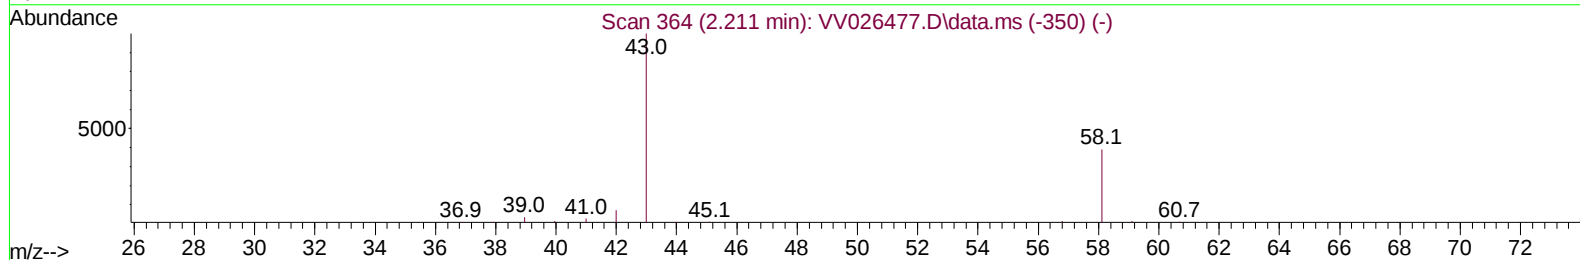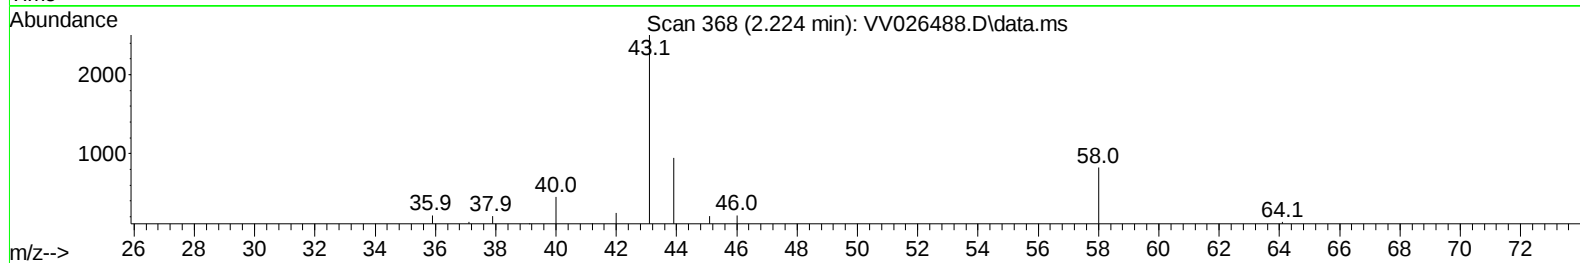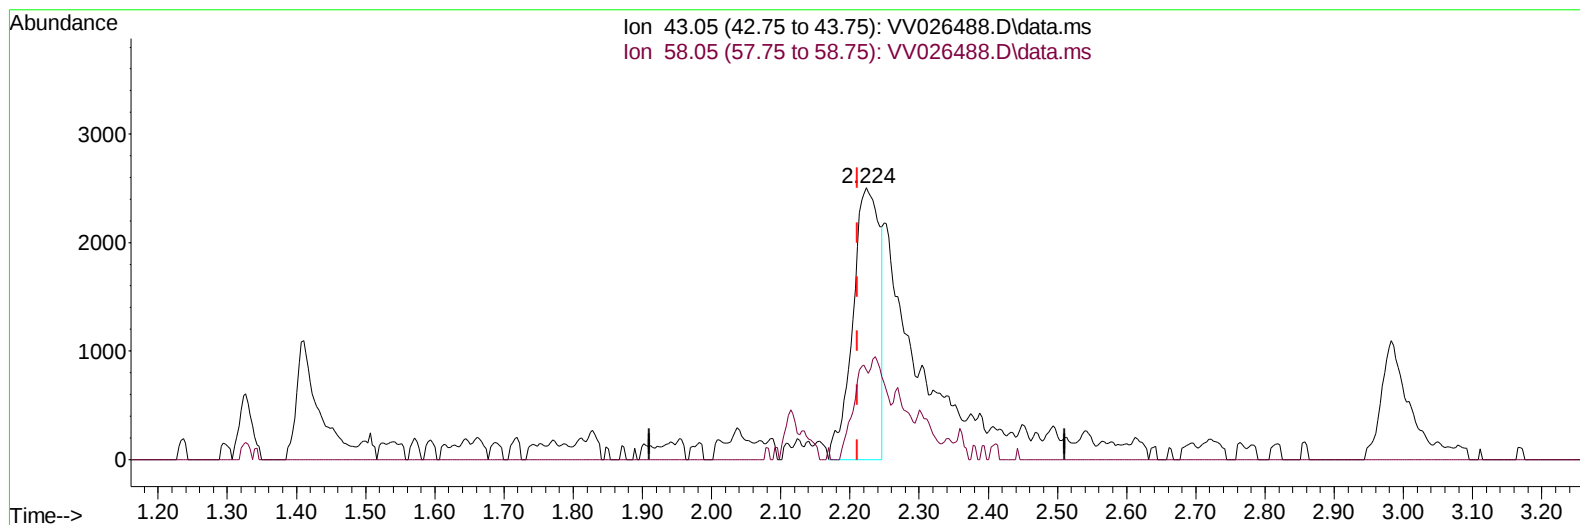

TIC: VV026488.D\data.ms

(13) Acetone (T)

2.224min (+ 0.013) 6.36 ug/L

response 6777

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	20.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026488.D
 Acq On : 21 Jun 2022 15:06
 Operator : SY/MD
 Sample : N3355-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C4

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:43:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

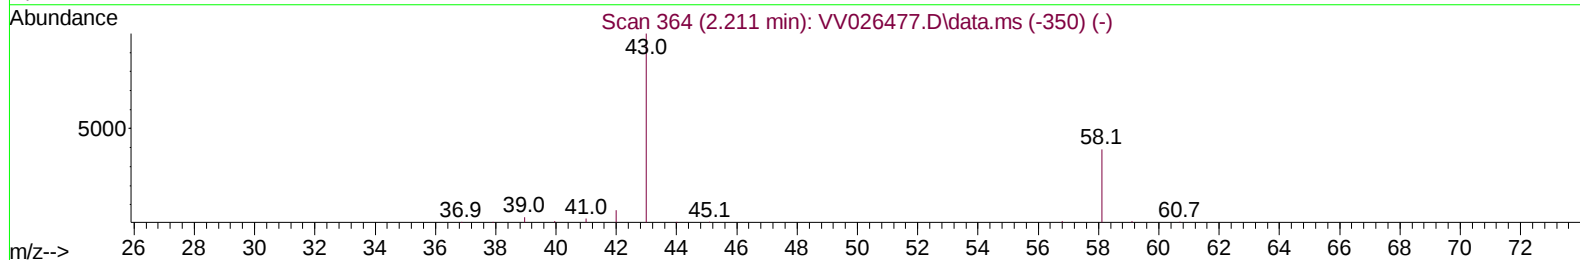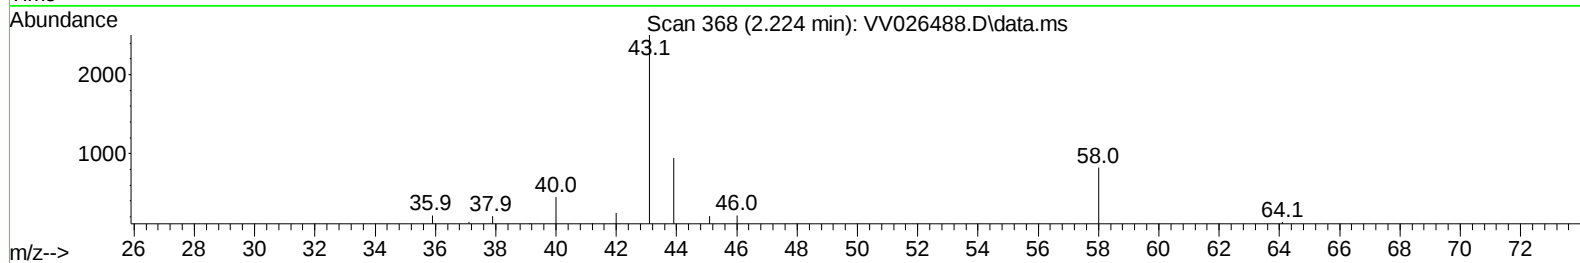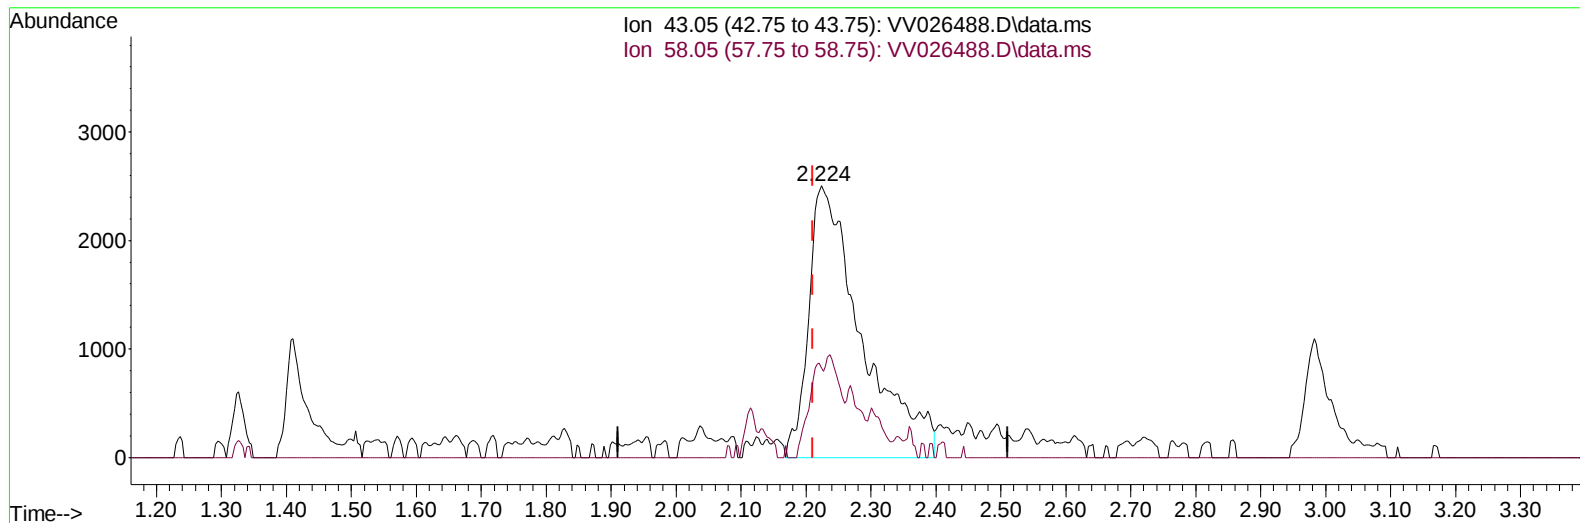

TIC: VV026488.D\data.ms

(13) Acetone (T)

2.224min (+ 0.013) 13.31 ug/L m

response 14190

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	9.73
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026488.D
 Acq On : 21 Jun 2022 15:06
 Operator : SY/MD
 Sample : N3355-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C4

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:43:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.629	114	162330	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	155524	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64324	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.327	65	59299	4.206	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	84.200%	
7) Chloroethane-d5	1.587	69	52141	4.703	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	94.000%	
11) 1,1-Dichloroethene-d2	2.127	63	88177	3.642	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	72.800%	
20) 2-Butanone-d5	3.934	46	73500	53.424	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	106.840%	
24) Chloroform-d	4.368	84	120369	5.825	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	116.400%	
26) 1,2-Dichloroethane-d4	5.047	65	48855	5.588	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	111.800%	
32) Benzene-d6	5.063	84	229886	5.529	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	110.600%	
36) 1,2-Dichloropropane-d6	6.079	67	69465	5.724	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	114.400%	
41) Toluene-d8	7.320	98	188291	4.966	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.400%	
43) trans-1,3-Dichloroprop...	7.632	79	16762	4.260	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	85.200%	
46) 2-Hexanone-d5	8.095	63	64461	54.229	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	108.460%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45242	6.052	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	121.000%#	
66) 1,2-Dichlorobenzene-d4	11.625	152	61846	6.242	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	124.800%#	
Target Compounds						
3) Chloromethane	1.259	50	12320	0.914	ug/L	95
13) Acetone	2.224	43	14190m	13.309	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026488.D
Acq On : 21 Jun 2022 15:06
Operator : SY/MD
Sample : N3355-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C4

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:43:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

