




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026491.D
 Acq On : 21 Jun 2022 16:14
 Operator : SY/MD
 Sample : N3355-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C9

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:43:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

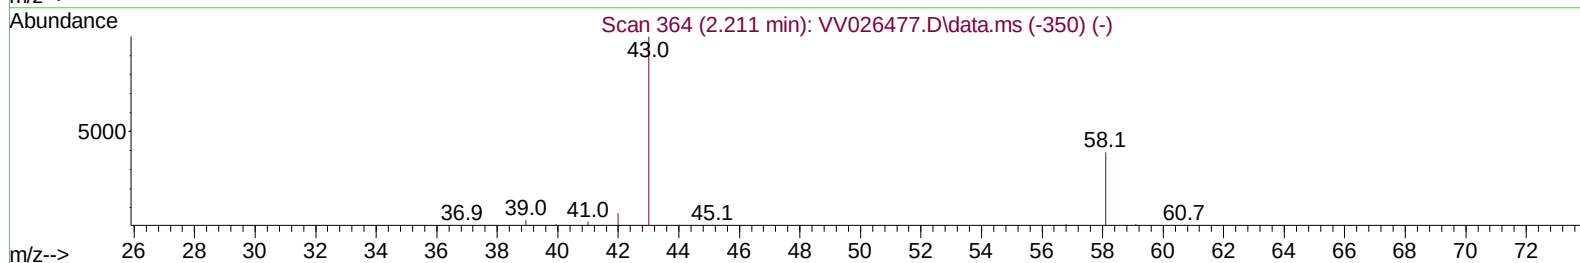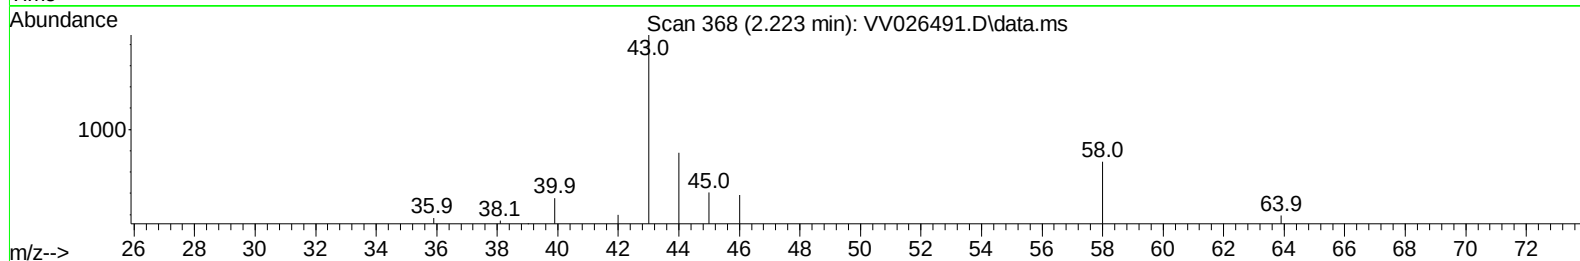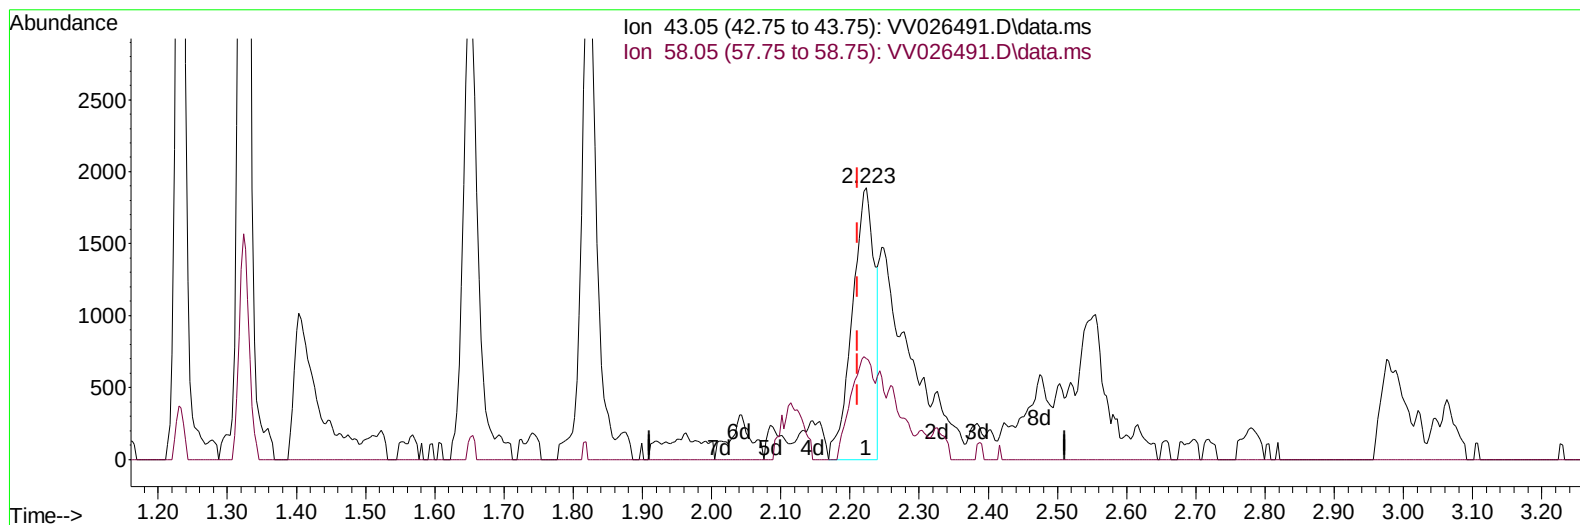

TIC: VV026491.D\data.ms

(13) Acetone (T)

2.223min (+ 0.013) 3.61 ug/L

response 4207

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	38.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026491.D
 Acq On : 21 Jun 2022 16:14
 Operator : SY/MD
 Sample : N3355-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C9

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:43:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

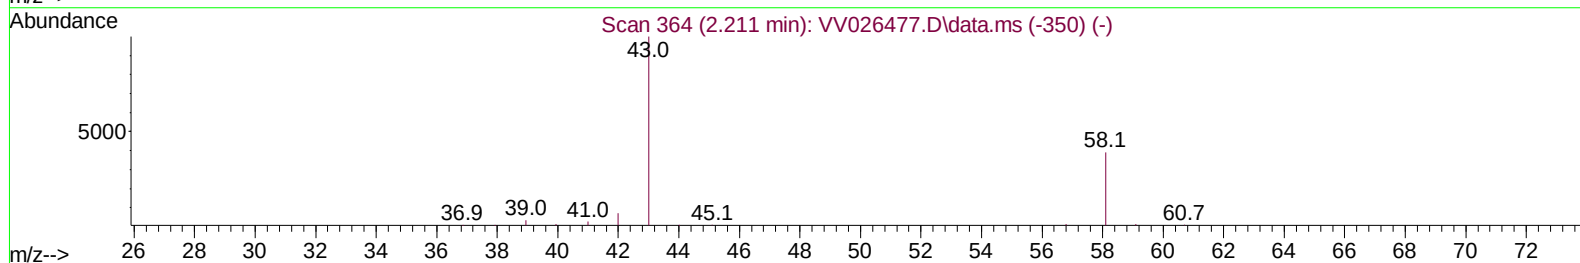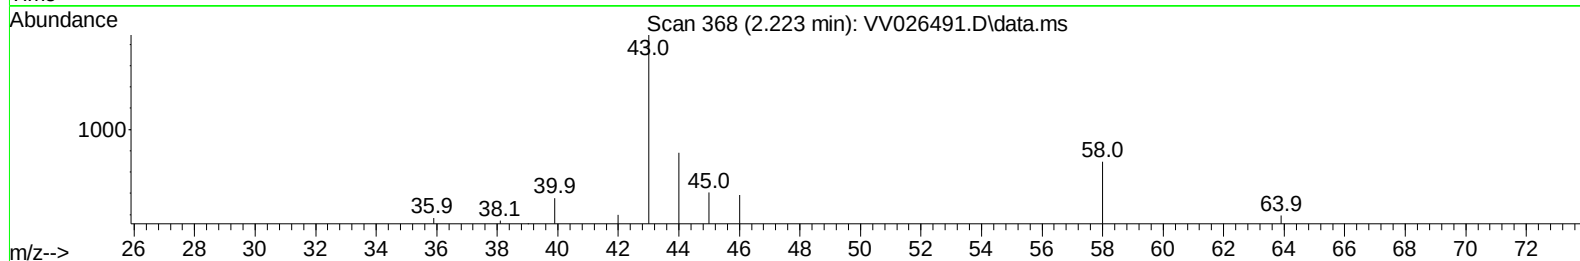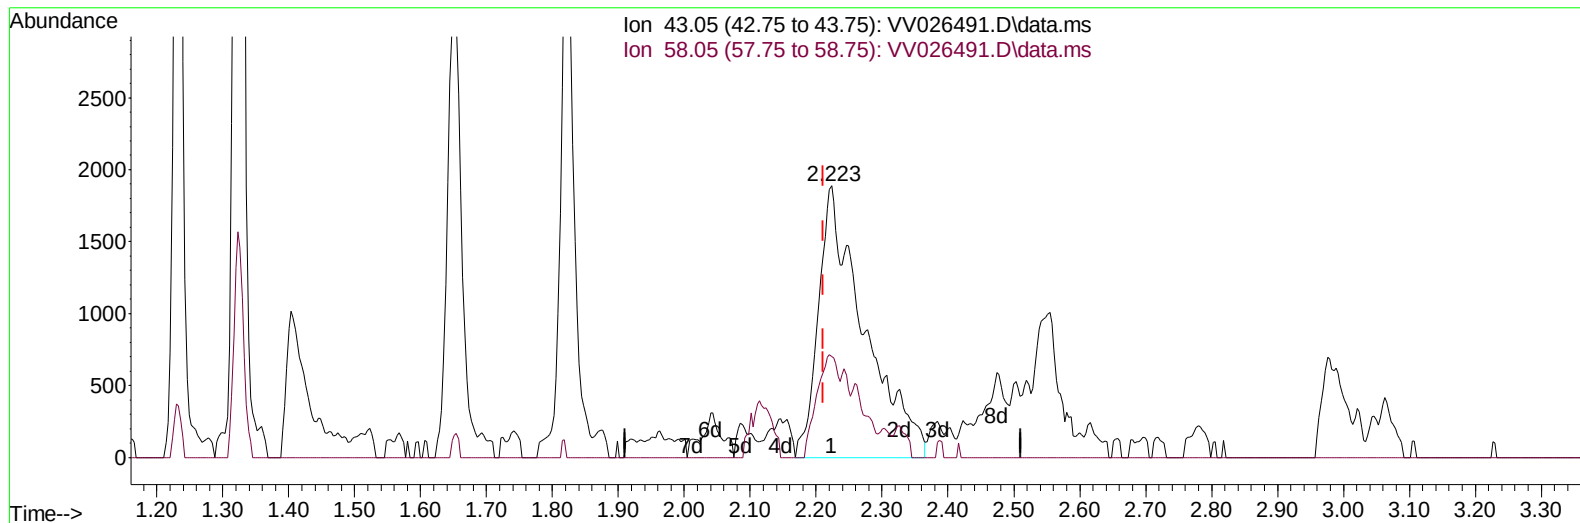

TIC: VV026491.D\data.ms

(13) Acetone (T)

2.223min (+ 0.013) 7.74 ug/L m

response 9024

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	17.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026491.D
 Acq On : 21 Jun 2022 16:14
 Operator : SY/MD
 Sample : N3355-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C9

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:43:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.628	114	177596	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	172076	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70590	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	56402	3.656	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	73.200%	
7) Chloroethane-d5	1.584	69	51031	4.207	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	84.200%	
11) 1,1-Dichloroethene-d2	2.124	63	83577	3.155	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	63.200%	
20) 2-Butanone-d5	3.937	46	77593	51.551	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	103.100%	
24) Chloroform-d	4.368	84	113681	5.028	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.600%	
26) 1,2-Dichloroethane-d4	5.046	65	47621	4.979	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.600%	
32) Benzene-d6	5.066	84	218664	4.753	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	95.000%	
36) 1,2-Dichloropropane-d6	6.079	67	69394	5.168	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	103.400%	
41) Toluene-d8	7.320	98	179255	4.273	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	85.400%	
43) trans-1,3-Dichloroprop...	7.632	79	15720	3.611	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	72.200%	
46) 2-Hexanone-d5	8.095	63	59633	45.342	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	90.680%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44005	5.320	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	106.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	58651	5.394	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	107.800%	
Target Compounds						
3) Chloromethane	1.259	50	4328	0.294	ug/L	97
13) Acetone	2.223	43	9024m	7.736	ug/L	
29) 1,1,1-Trichloroethane	4.628	97	3751	0.197	ug/L #	87
34) Trichloroethene	5.924	95	112057	9.304	ug/L	98
52) Ethylbenzene	9.024	91	2368	0.051	ug/L	90
53) m,p-Xylene	9.146	106	1987	0.110	ug/L	81
63) 1,2,4-Trimethylbenzene	10.918	105	2603	0.088	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026491.D
Acq On : 21 Jun 2022 16:14
Operator : SY/MD
Sample : N3355-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C9

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:43:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

