




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026493.D
Acq On : 21 Jun 2022 17:02
Operator : SY/MD
Sample : N3355-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D1

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:44:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

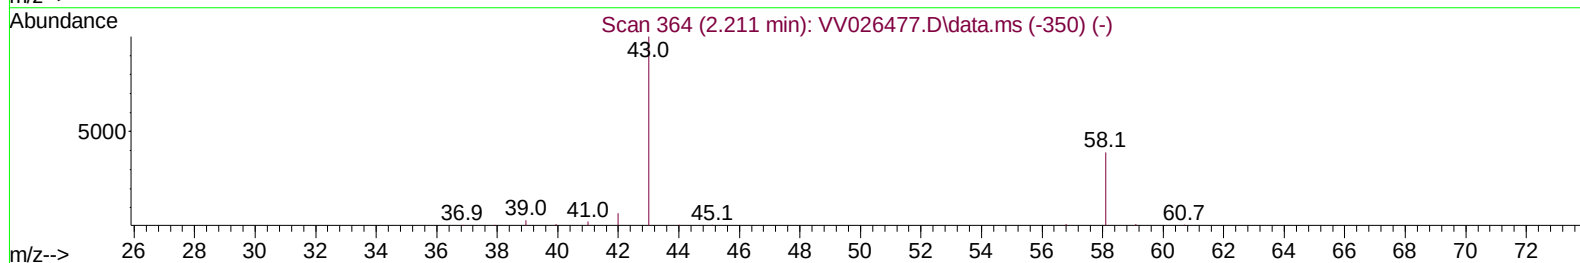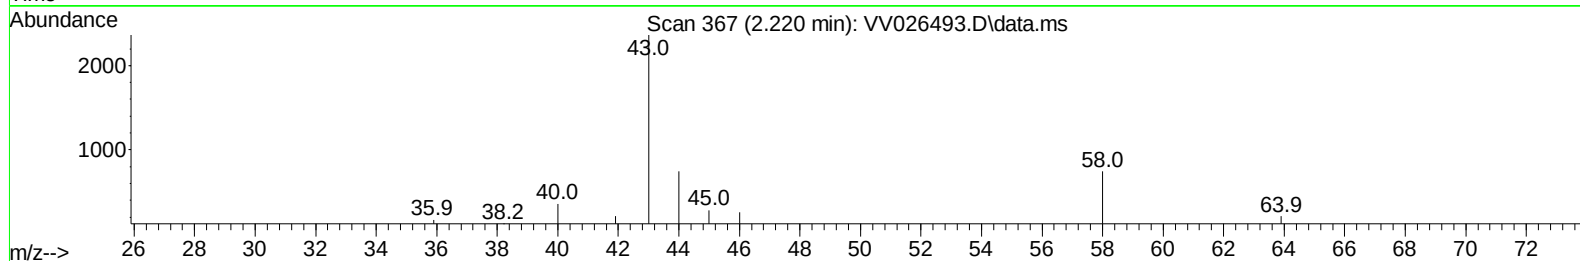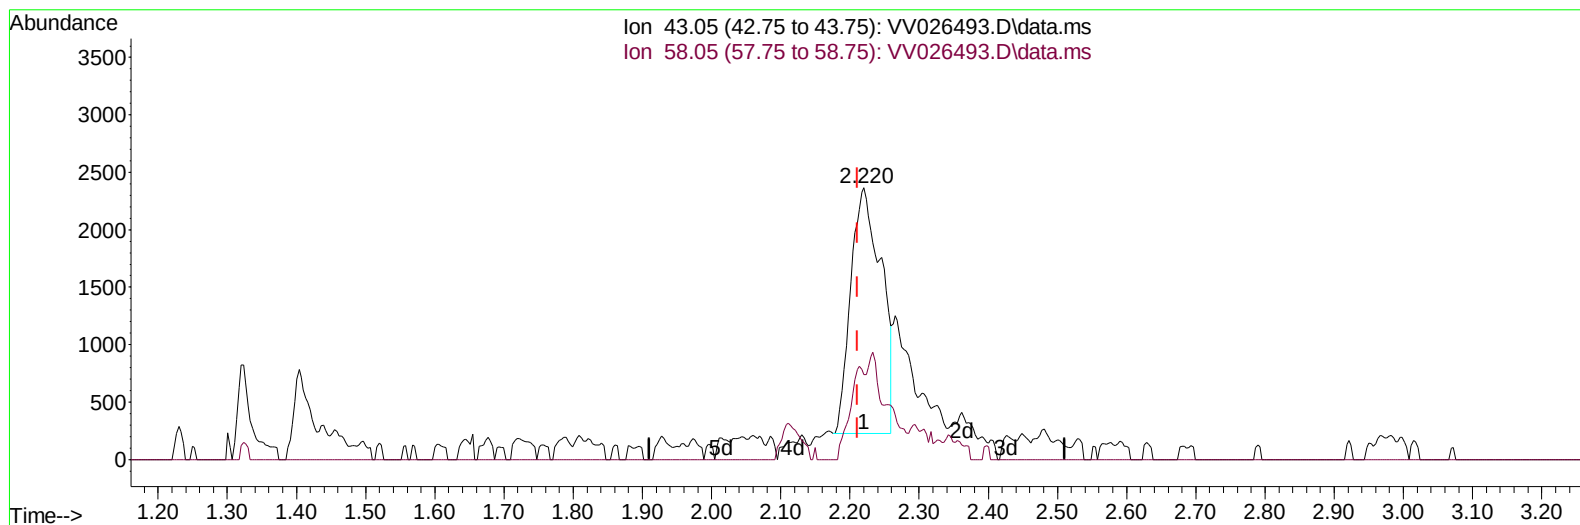

TIC: VV026493.D\data.ms

(13) Acetone (T)

2.220min (+ 0.010) 6.33 ug/L

response 6521

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	20.13
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026493.D
 Acq On : 21 Jun 2022 17:02
 Operator : SY/MD
 Sample : N3355-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:44:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

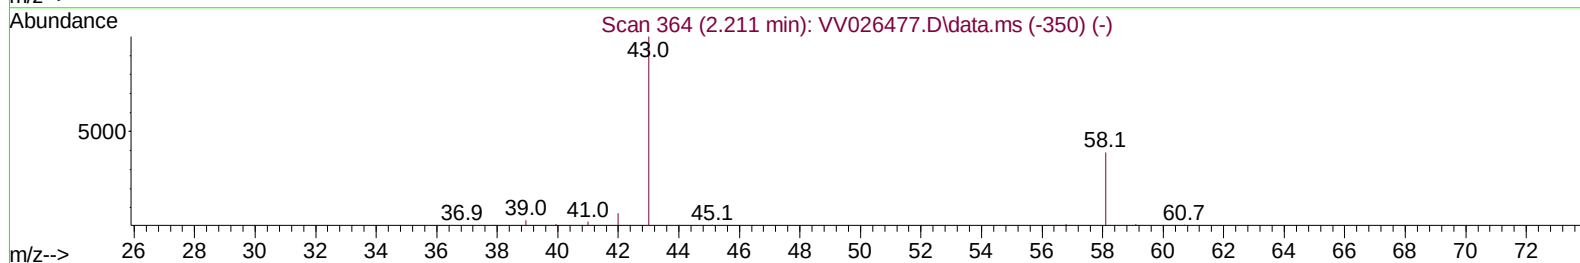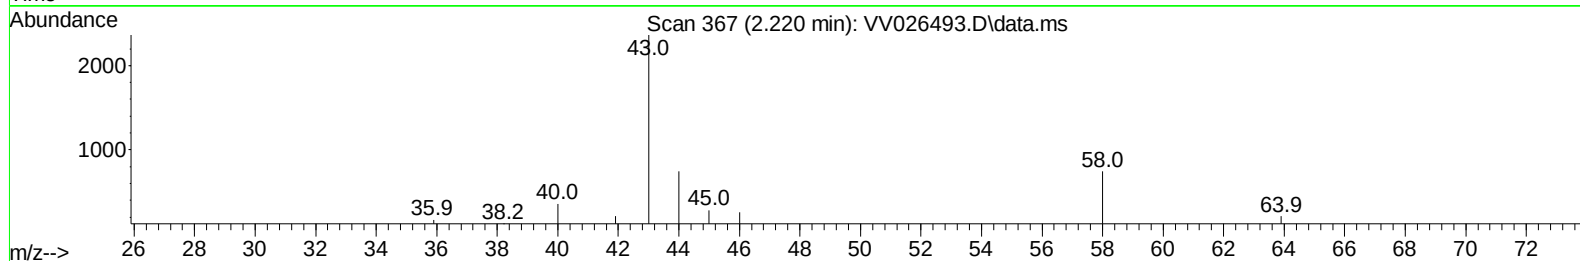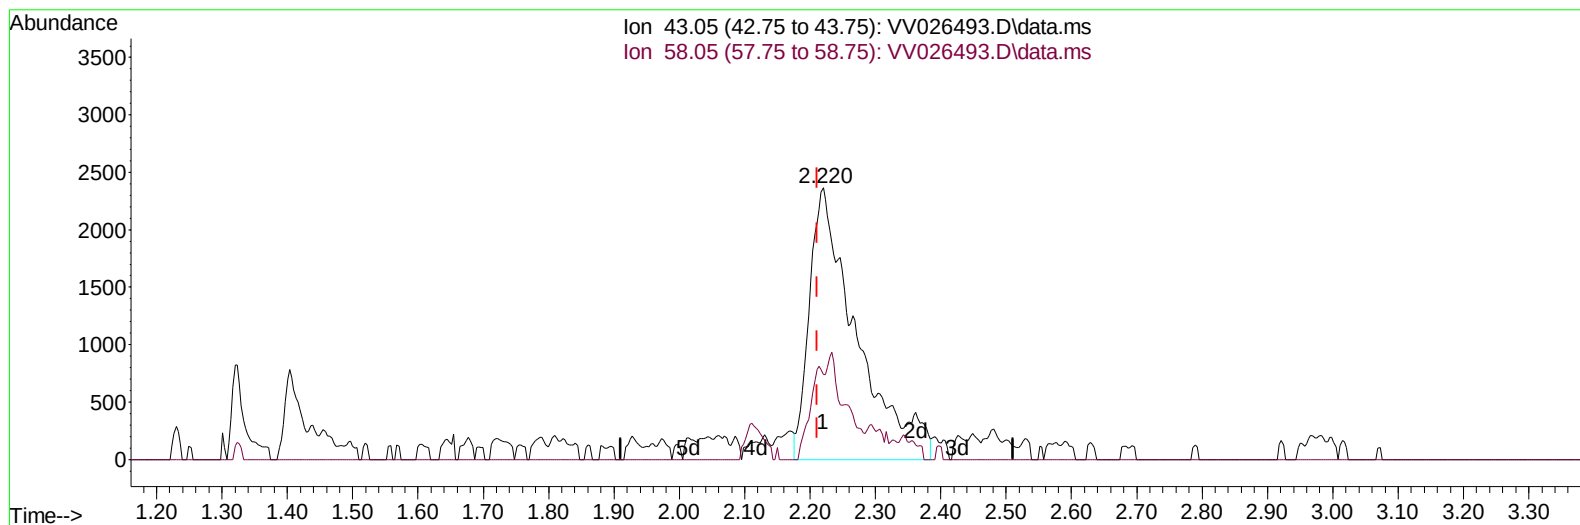

TIC: VV026493.D\data.ms

(13) Acetone (T)

2.220min (+ 0.010) 11.45 ug/L m

response 11785

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	11.14
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026493.D
 Acq On : 21 Jun 2022 17:02
 Operator : SY/MD
 Sample : N3355-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:44:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.625	114		156764	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		152536	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		60734	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.323	65		54005	3.966	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.400%	
7) Chloroethane-d5	1.584	69		49738	4.646	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%	
11) 1,1-Dichloroethene-d2	2.121	63		80279	3.433	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%	
20) 2-Butanone-d5	3.928	46		74788	56.291	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.580%	
24) Chloroform-d	4.362	84		112570	5.641	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.800%	
26) 1,2-Dichloroethane-d4	5.047	65		46241	5.477	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.600%	
32) Benzene-d6	5.063	84		208775	5.119	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%	
36) 1,2-Dichloropropane-d6	6.079	67		65211	5.479	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.600%	
41) Toluene-d8	7.320	98		172442	4.637	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	7.632	79		13688	3.547	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.000%	
46) 2-Hexanone-d5	8.095	63		57924	49.684	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.360%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		41801	5.701	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152		56697	6.061	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	121.200%#	
Target Compounds							
13) Acetone	2.220	43		11785m	11.446	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026493.D
Acq On : 21 Jun 2022 17:02
Operator : SY/MD
Sample : N3355-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:44:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

