




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026494.D
 Acq On : 21 Jun 2022 17:26
 Operator : SY/MD
 Sample : N3355-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D2

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:44:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

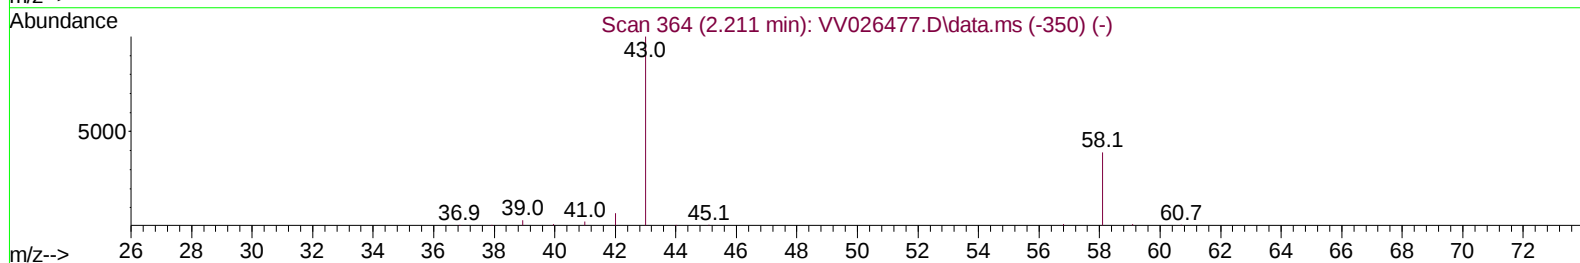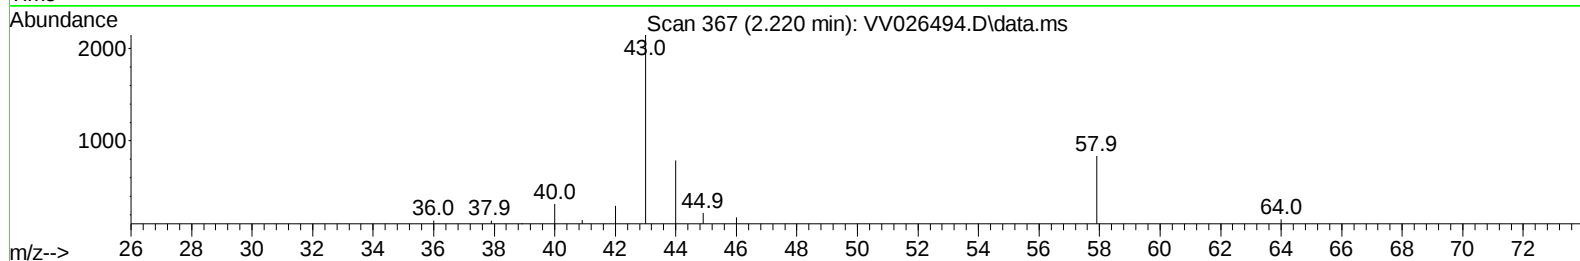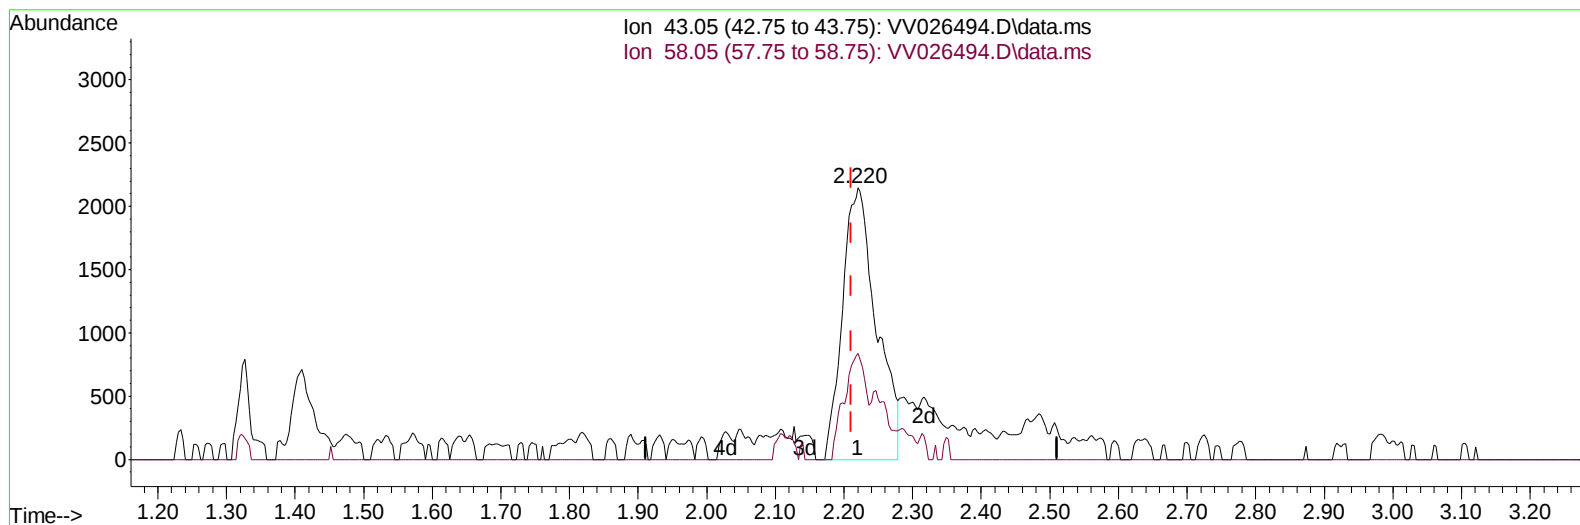

TIC: VV026494.D\data.ms

(13) Acetone (T)

2.220min (+ 0.010) 6.87 ug/L

response 7364

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	24.96
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026494.D
 Acq On : 21 Jun 2022 17:26
 Operator : SY/MD
 Sample : N3355-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D2

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:44:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

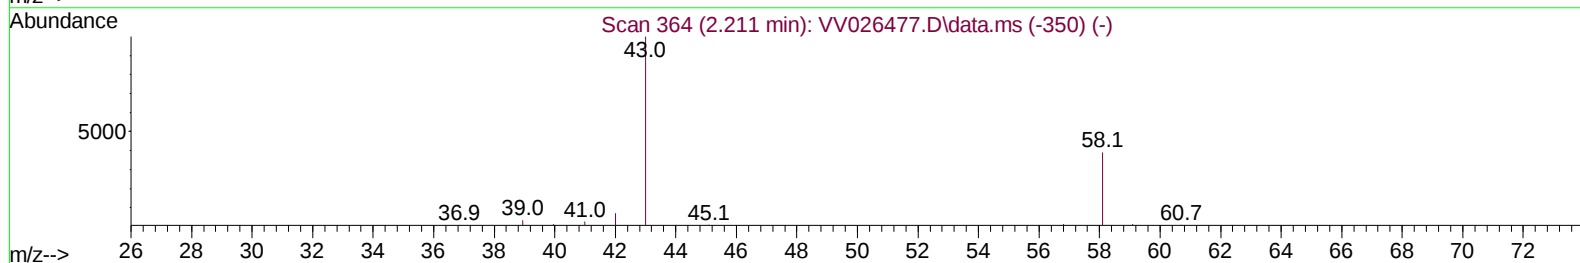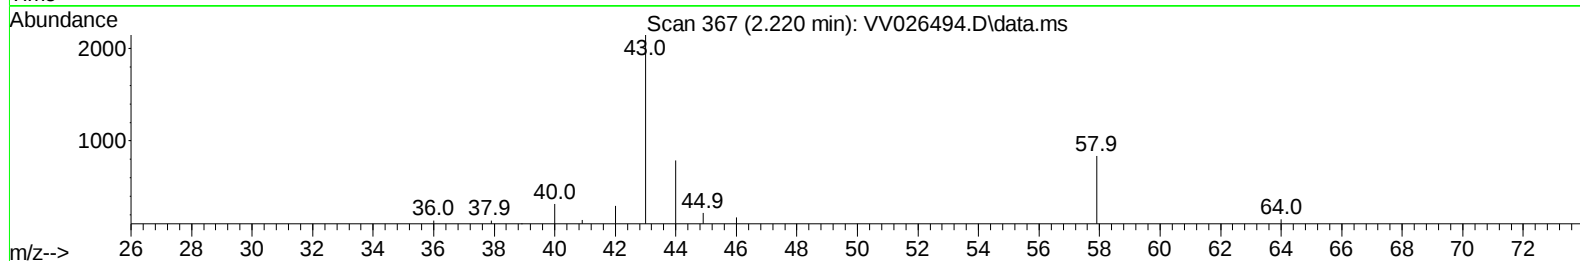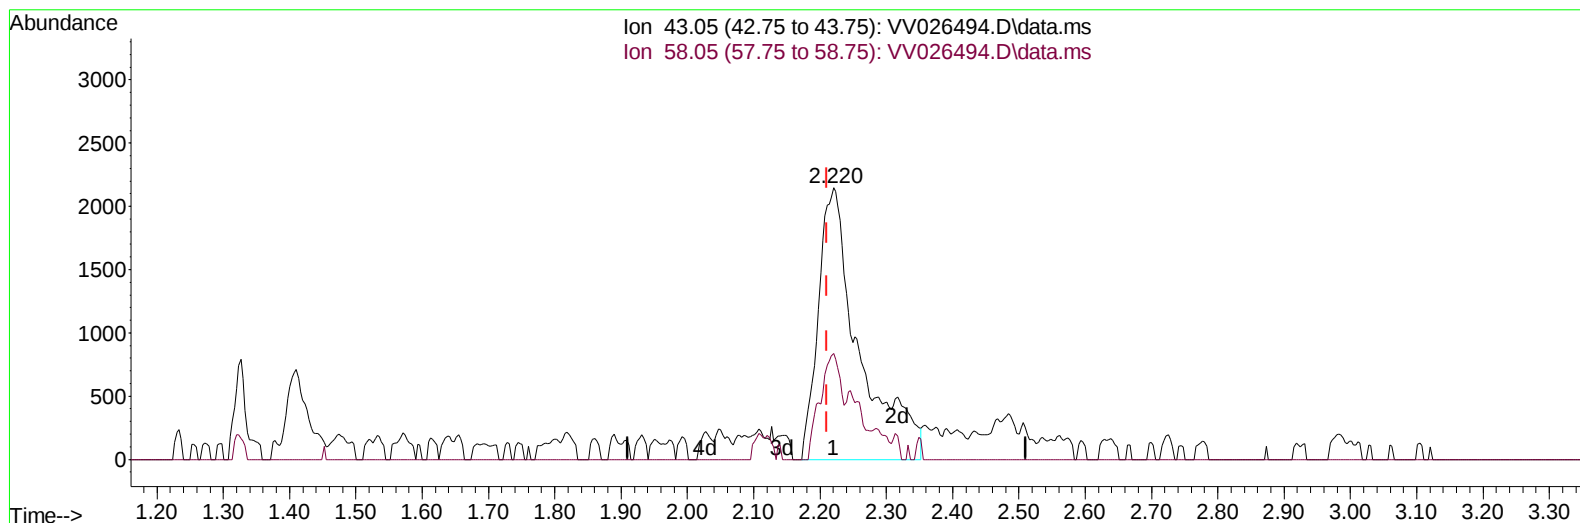

TIC: VV026494.D\data.ms

(13) Acetone (T)

2.220min (+ 0.010) 8.54 ug/L m

response 9145

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	20.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026494.D
 Acq On : 21 Jun 2022 17:26
 Operator : SY/MD
 Sample : N3355-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D2

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:44:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.629	114		163124	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		156469	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		63662	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.323	65		53546	3.779	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.600%	
7) Chloroethane-d5	1.584	69		50944	4.573	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.400%	
11) 1,1-Dichloroethene-d2	2.124	63		81588	3.353	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.000%	
20) 2-Butanone-d5	3.925	46		69199	50.053	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.100%	
24) Chloroform-d	4.365	84		115596	5.566	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.400%	
26) 1,2-Dichloroethane-d4	5.047	65		44750	5.093	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.800%	
32) Benzene-d6	5.063	84		213567	5.105	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.200%	
36) 1,2-Dichloropropane-d6	6.079	67		65417	5.358	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.200%	
41) Toluene-d8	7.320	98		174029	4.562	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%	
43) trans-1,3-Dichloroprop...	7.632	79		13846	3.497	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.000%	
46) 2-Hexanone-d5	8.095	63		56294	47.073	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.140%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		43486	5.782	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152		58711	5.987	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.800%	
Target Compounds							
3) Chloromethane	1.259	50		2531	0.187	ug/L	95
13) Acetone	2.220	43		9145m	8.536	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026494.D
Acq On : 21 Jun 2022 17:26
Operator : SY/MD
Sample : N3355-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D2

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:44:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

