




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026497.D
Acq On : 21 Jun 2022 18:38
Operator : SY/MD
Sample : N3355-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C8

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:45:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

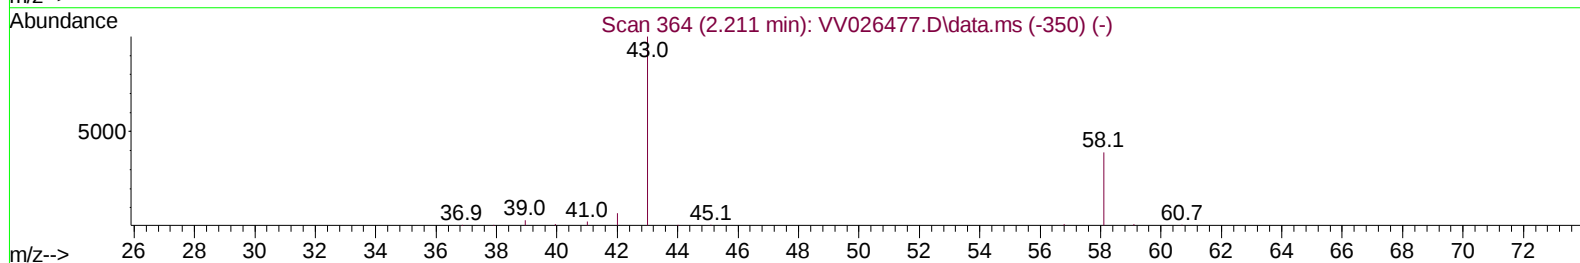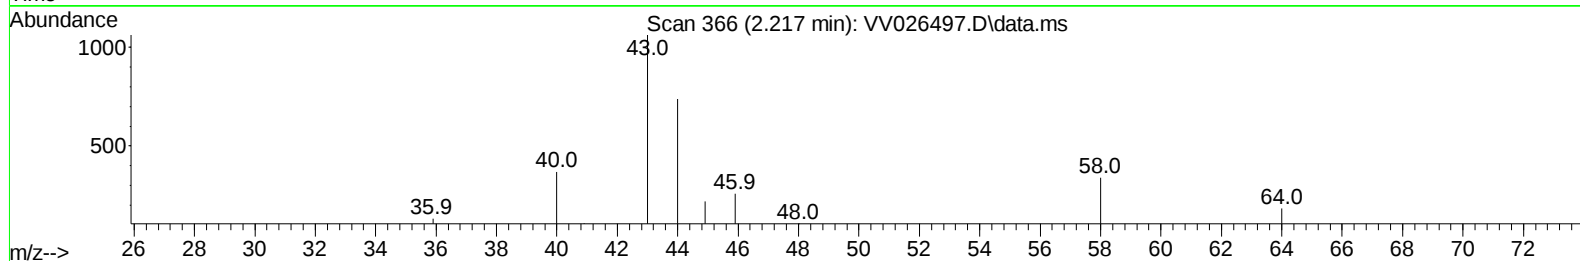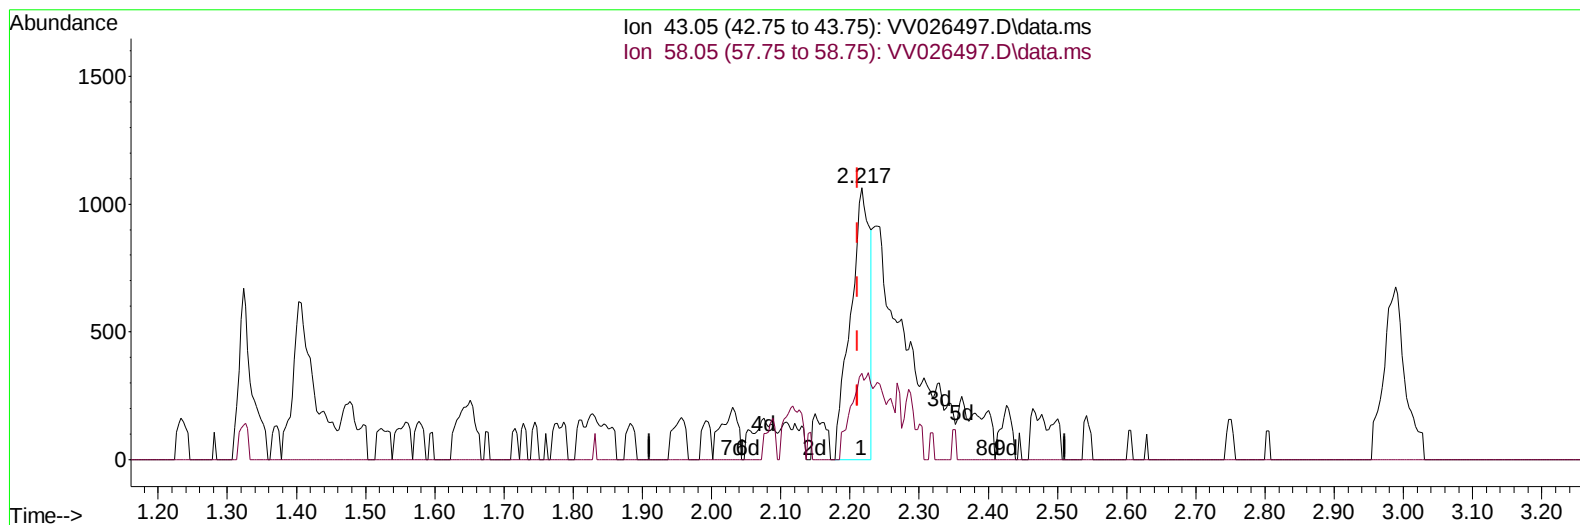

TIC: VV026497.D\data.ms

(13) Acetone (T)

2.217min (+ 0.006) 1.96 ug/L

response	2021	
Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	34.98
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026497.D
 Acq On : 21 Jun 2022 18:38
 Operator : SY/MD
 Sample : N3355-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:45:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

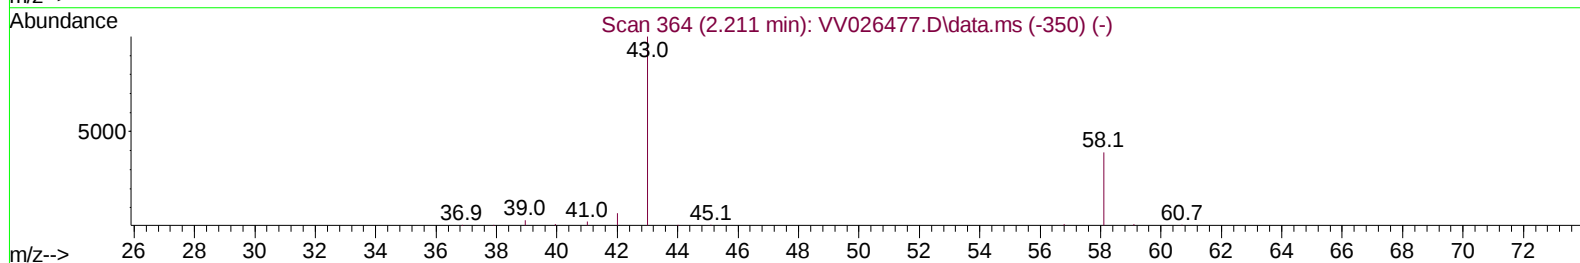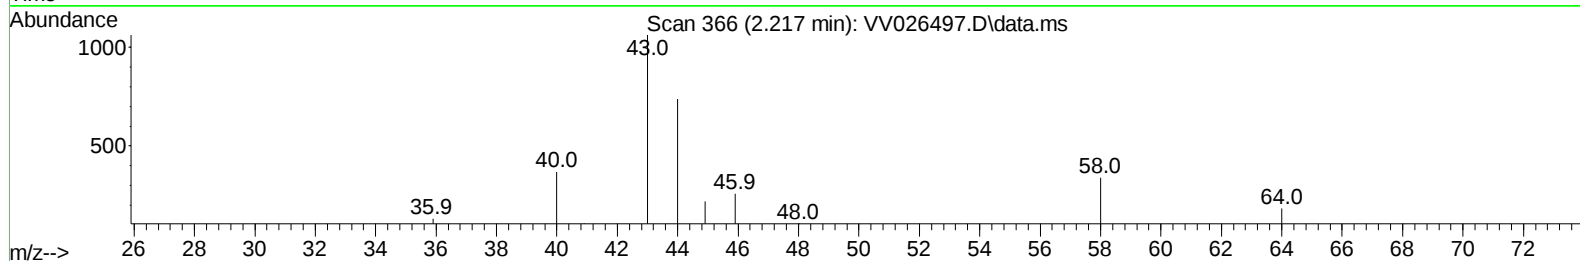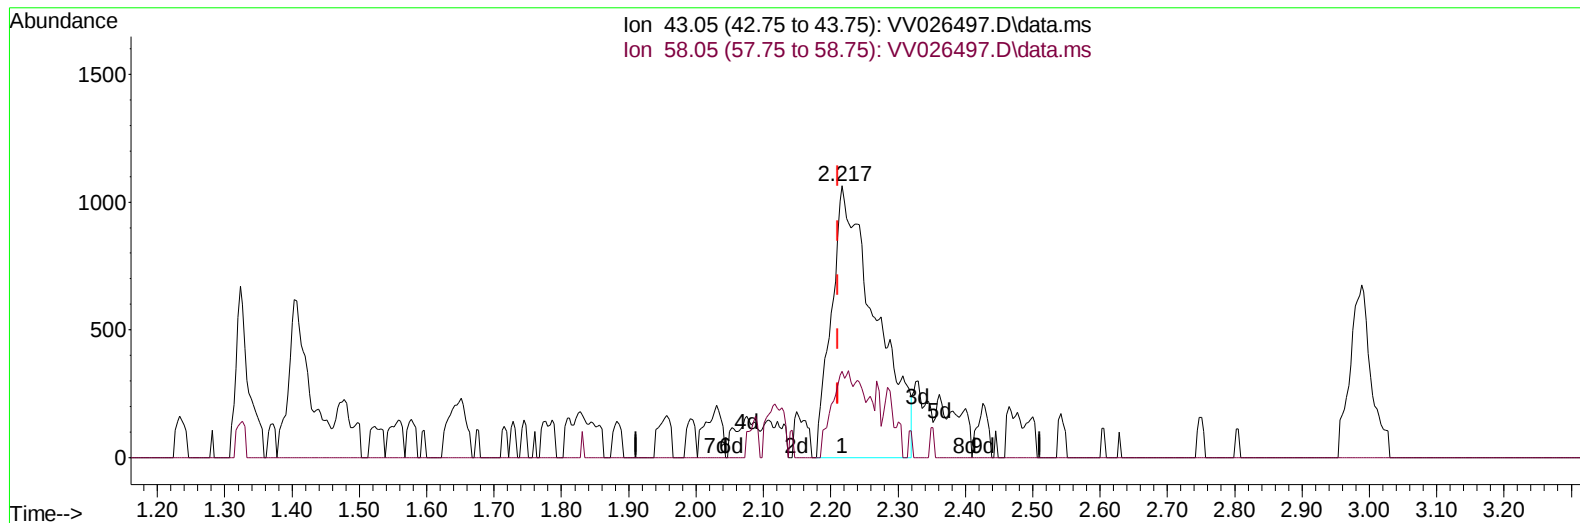

TIC: VV026497.D\data.ms

(13) Acetone (T)

2.217min (+ 0.006) 4.69 ug/L m

response 4827

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	14.65
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026497.D
 Acq On : 21 Jun 2022 18:38
 Operator : SY/MD
 Sample : N3355-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:45:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	156616	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	151772	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61417	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	55906	4.110	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	82.200%	
7) Chloroethane-d5	1.584	69	51661	4.830	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	96.600%	
11) 1,1-Dichloroethene-d2	2.124	63	83357	3.568	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	71.400%	
20) 2-Butanone-d5	3.931	46	77897	58.686	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	117.380%	
24) Chloroform-d	4.365	84	118358	5.936	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	118.800%	
26) 1,2-Dichloroethane-d4	5.046	65	46604	5.525	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	110.400%	
32) Benzene-d6	5.063	84	218407	5.383	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	107.600%	
36) 1,2-Dichloropropane-d6	6.079	67	70646	5.966	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	119.400%	
41) Toluene-d8	7.320	98	180157	4.869	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	97.400%	
43) trans-1,3-Dichloroprop...	7.628	79	14913	3.884	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	77.600%	
46) 2-Hexanone-d5	8.095	63	61299	52.844	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	105.680%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43714	5.992	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	119.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60379	6.382	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	127.600%#	
Target Compounds						
13) Acetone	2.217	43	4827m	4.693	ug/L	
29) 1,1,1-Trichloroethane	4.625	97	21083	1.257	ug/L	99
34) Trichloroethene	5.918	95	647733	60.974	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026497.D
Acq On : 21 Jun 2022 18:38
Operator : SY/MD
Sample : N3355-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:45:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

