




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026499.D
 Acq On : 21 Jun 2022 19:26
 Operator : SY/MD
 Sample : N3374-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S6

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:45:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

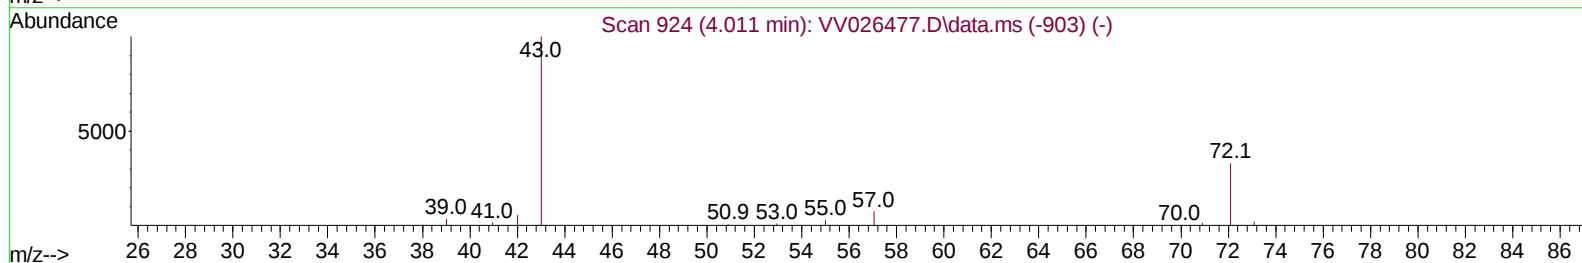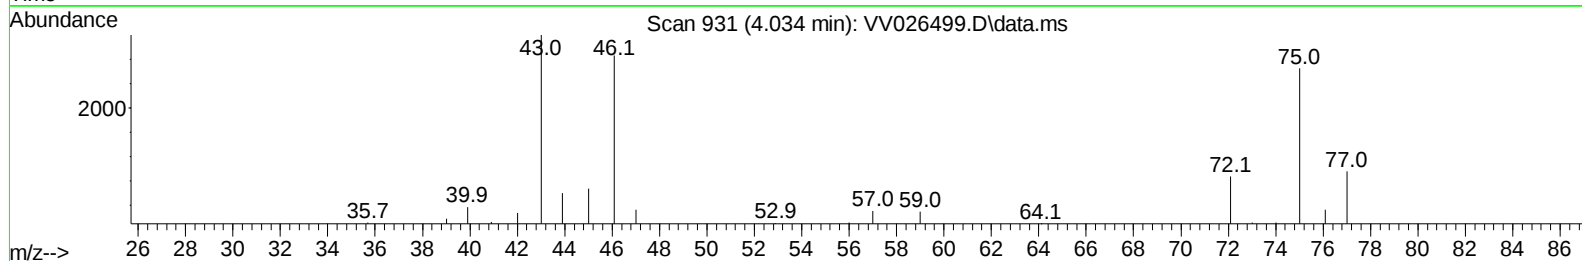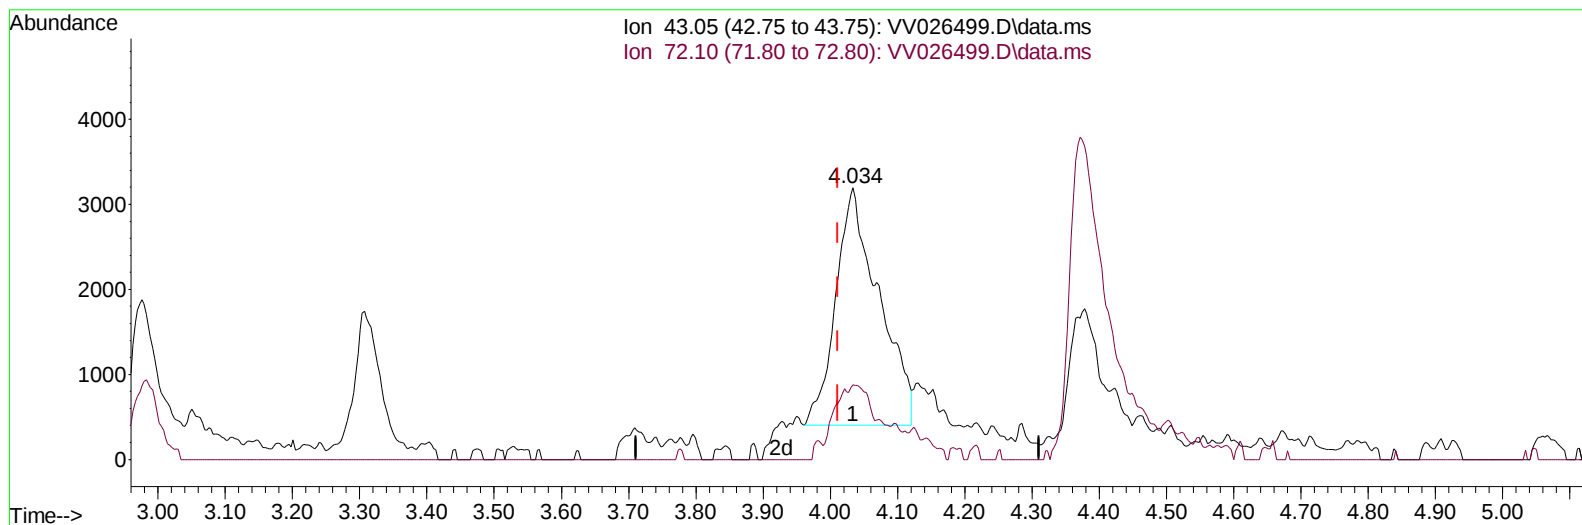

TIC: VV026499.D\data.ms

(21) 2-Butanone (T)

4.034min (+ 0.022) 8.17 ug/L

response 12421

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	24.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026499.D
 Acq On : 21 Jun 2022 19:26
 Operator : SY/MD
 Sample : N3374-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S6

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:45:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

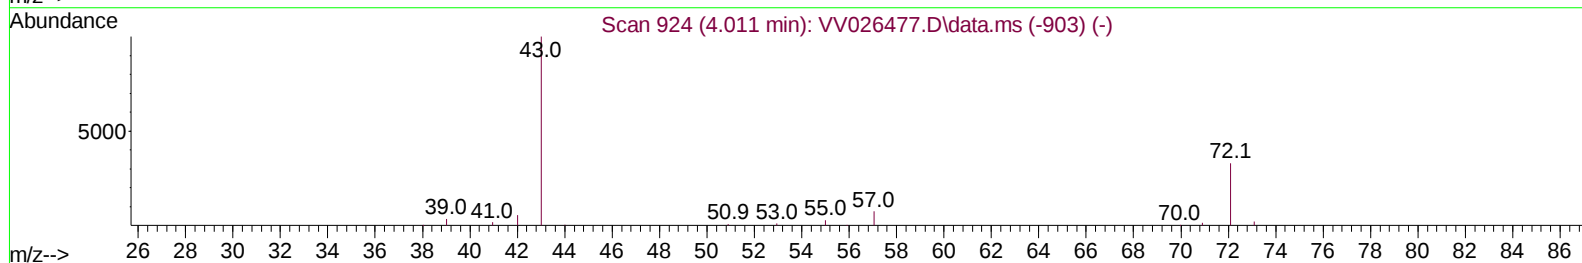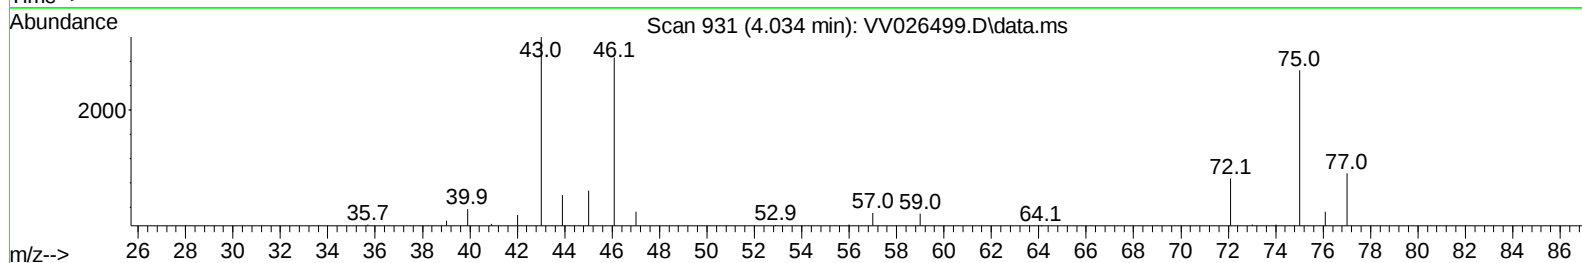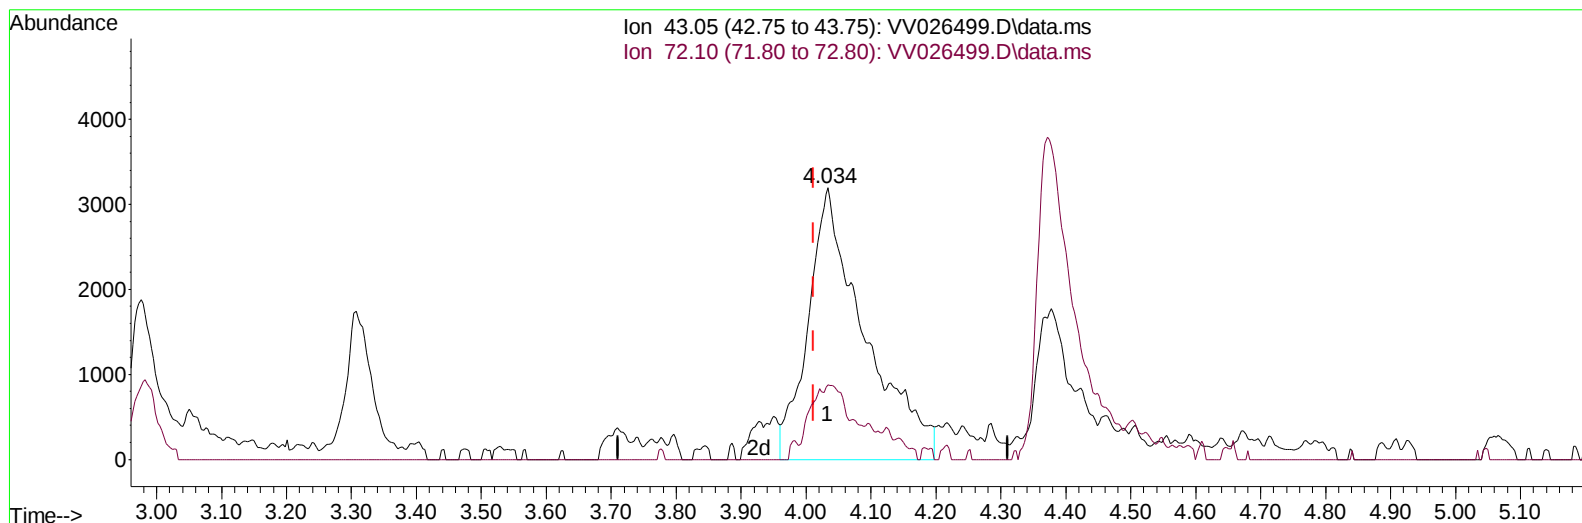

TIC: VV026499.D\data.ms

(21) 2-Butanone (T)

4.034min (+ 0.022) 12.63 ug/L m

response 19212

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	15.76
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026499.D
 Acq On : 21 Jun 2022 19:26
 Operator : SY/MD
 Sample : N3374-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S6

Manual IntegrationsAPPROVED

Quant Time: Jun 22 04:45:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	178984	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	171304	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	94019	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	57473	3.697	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	74.000%	
7) Chloroethane-d5	1.584	69	50908	4.165	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	83.200%	
11) 1,1-Dichloroethene-d2	2.124	63	82830	3.103	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	62.000%	
20) 2-Butanone-d5	3.931	46	72977	48.109	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	96.220%	
24) Chloroform-d	4.365	84	118914	5.219	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	104.400%	
26) 1,2-Dichloroethane-d4	5.047	65	45223	4.691	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	93.800%	
32) Benzene-d6	5.063	84	226818	4.953	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	99.000%	
36) 1,2-Dichloropropane-d6	6.079	67	70211	5.253	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	105.000%	
41) Toluene-d8	7.320	98	200518	4.802	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	96.000%	
43) trans-1,3-Dichloroprop...	7.628	79	17224	3.974	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	79.400%	
46) 2-Hexanone-d5	8.091	63	76954	58.776	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	117.560%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47960	5.825	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	116.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	79630	5.499	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	110.000%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.150	85	3800	0.284	ug/L	99
13) Acetone	2.224	43	127561	108.509	ug/L	89
14) Carbon disulfide	2.310	76	44345	1.591	ug/L	97
19) 1,1-Dichloroethane	3.211	63	2466	0.118	ug/L #	91
21) 2-Butanone	4.034	43	19212m	12.630	ug/L	
30) Cyclohexane	4.690	56	1947	0.138	ug/L #	91
33) Benzene	5.114	78	54632	1.244	ug/L	100
35) Methylcyclohexane	6.143	83	921	0.056	ug/L #	49
40) 4-Methyl-2-pentanone	7.236	43	19199	4.546	ug/L #	88
42) Toluene	7.394	91	32849	0.711	ug/L	94
51) Chlorobenzene	8.886	112	3346	0.111	ug/L	93
52) Ethylbenzene	9.017	91	19731	0.426	ug/L	99
53) m,p-Xylene	9.143	106	12471	0.691	ug/L	88
54) o-Xylene	9.545	106	5366	0.307	ug/L	94
55) Styrene	9.574	104	1613	0.055	ug/L	89
60) Isopropylbenzene	9.931	105	27635	0.551	ug/L	99
62) 1,3,5-Trimethylbenzene	10.538	105	7251	0.182	ug/L	100
63) 1,2,4-Trimethylbenzene	10.915	105	17647	0.448	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026499.D
 Acq On : 21 Jun 2022 19:26
 Operator : SY/MD
 Sample : N3374-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S6

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:45:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026499.D
Acq On : 21 Jun 2022 19:26
Operator : SY/MD
Sample : N3374-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S6

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:45:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

