

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026478.D
 Acq On : 21 Jun 2022 10:59
 Operator : SY/MD
 Sample : VV0621WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK382

Quant Time: Jun 22 04:40:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	197528	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	188430	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77359	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	64104	3.736	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.800%
7) Chloroethane-d5	1.584	69	55262	4.097	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.000%
11) 1,1-Dichloroethene-d2	2.121	63	94953	3.223	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.400%
20) 2-Butanone-d5	3.928	46	73084	43.656	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.320%
24) Chloroform-d	4.359	84	125947	5.009	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
26) 1,2-Dichloroethane-d4	5.043	65	50567	4.753	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.000%
32) Benzene-d6	5.056	84	243582	4.835	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
36) 1,2-Dichloropropane-d6	6.072	67	74124	5.042	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.317	98	200439	4.364	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.629	79	18276	3.833	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.600%
46) 2-Hexanone-d5	8.092	63	67240	46.689	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.380%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	47348	5.228	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	64699	5.430	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.600%
Target Compounds						Qvalue
16) Methylene chloride	2.523	84	13194	0.829	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026478.D
Acq On : 21 Jun 2022 10:59
Operator : SY/MD
Sample : VV0621WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK382


Quant Time: Jun 22 04:40:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

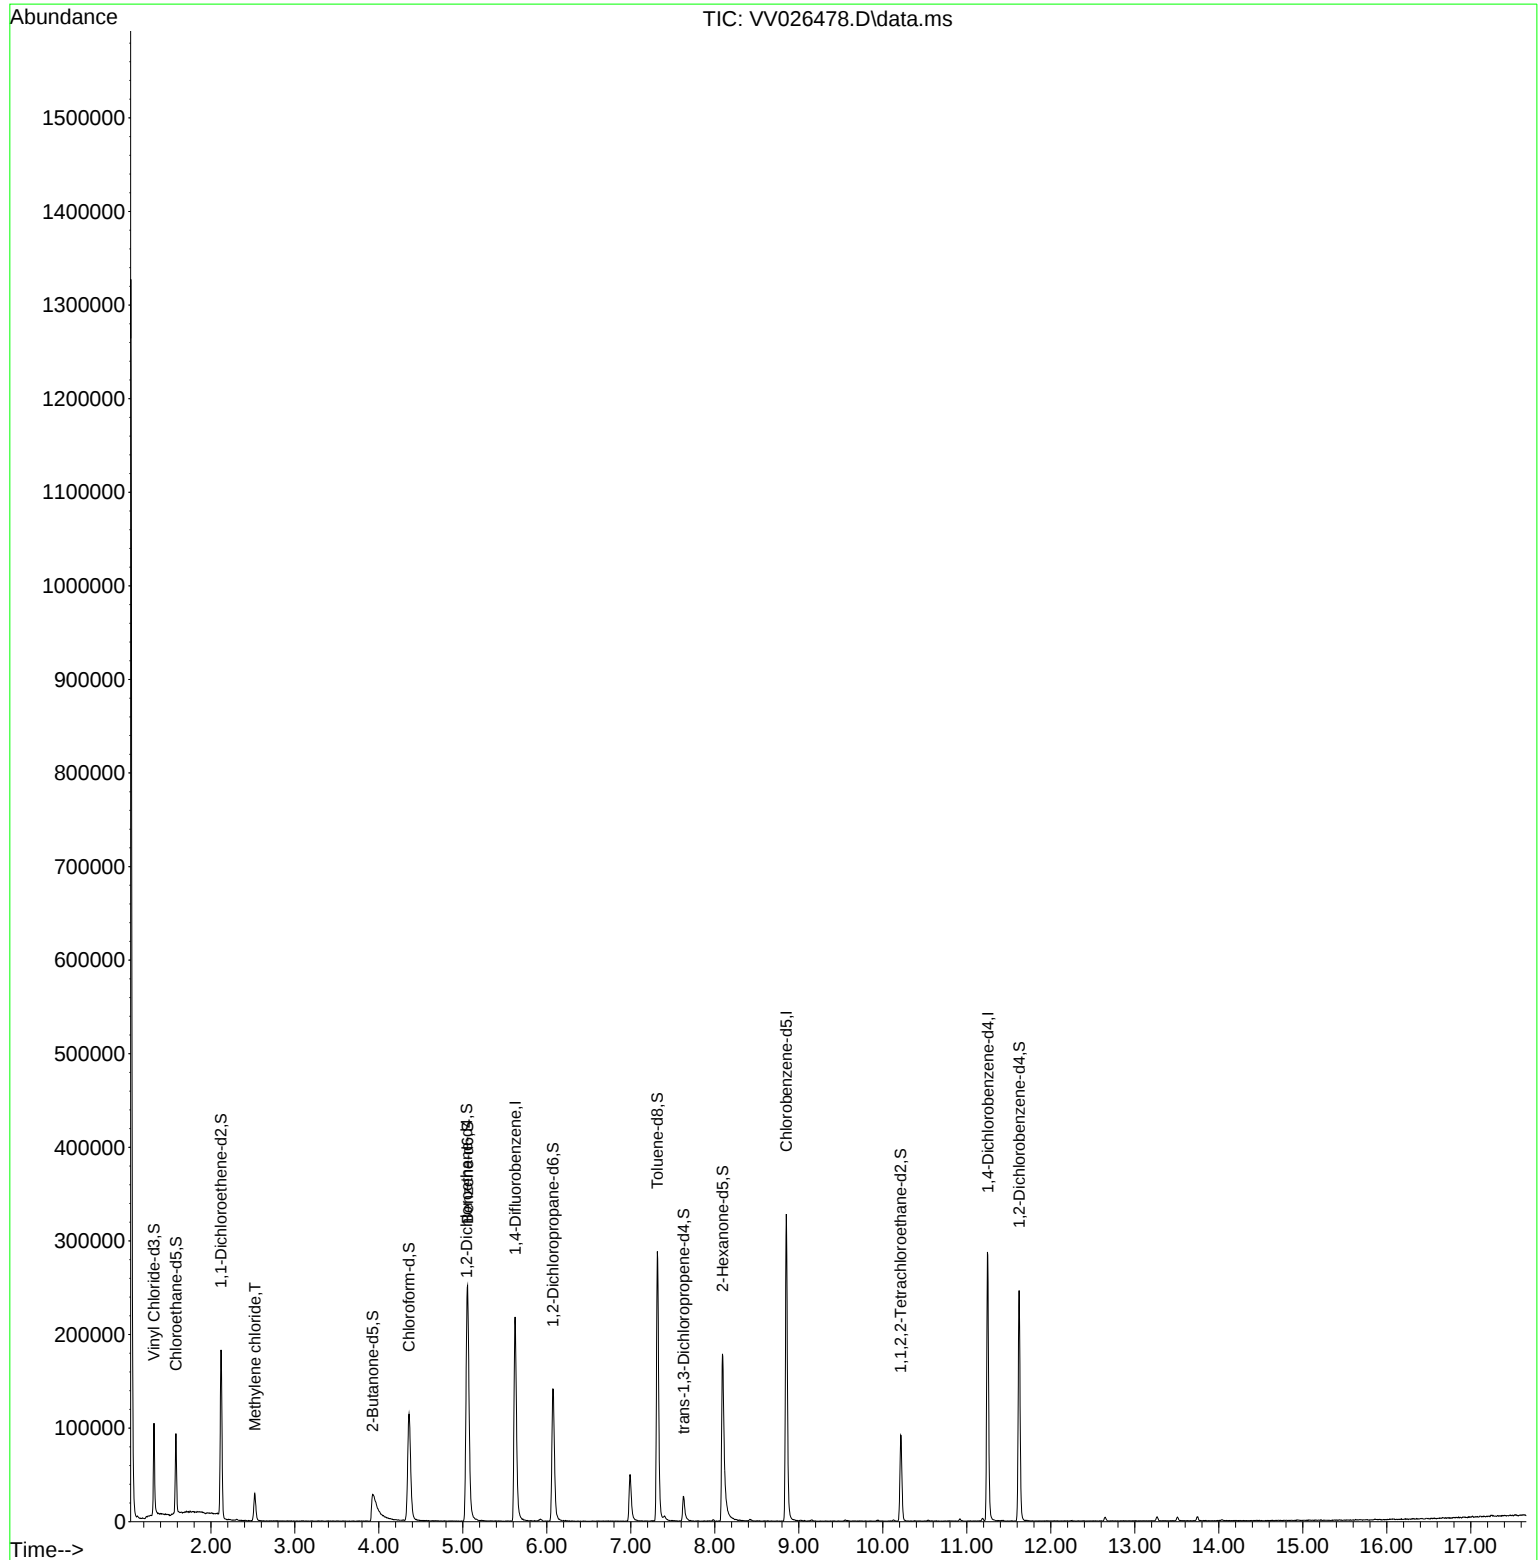

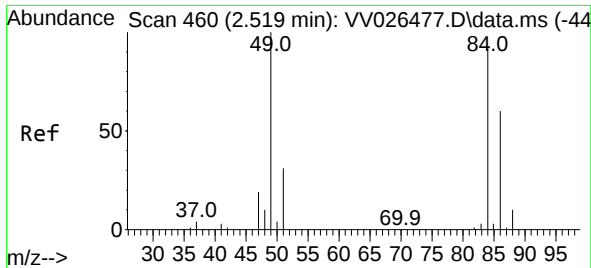

#16
Methylene chloride
Concen: 0.829 ug/L
RT: 2.523 min Scan# 461
Delta R.T. 0.003 min
Lab File: VV026478.D
Acq: 21 Jun 2022 10:59

Instrument :
MSVOA_V
ClientSampleId :
VBLK382

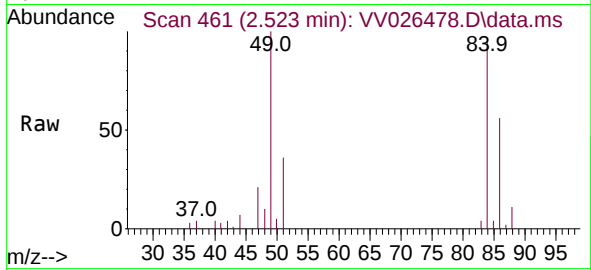

Tgt Ion: 84 Resp: 13194
Ion Ratio Lower Upper
84 100
86 59.4 44.0 81.8
49 105.5 77.3 143.7

