

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062122\
 Data File : VW026485.D
 Acq On : 21 Jun 2022 13:56
 Operator : SY/MD
 Sample : N3358-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 22 04:42:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	181991	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	177796	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72238	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	62556	3.957	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.200%	
7) Chloroethane-d5	1.584	69	56259	4.526	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.600%	
11) 1,1-Dichloroethene-d2	2.124	63	93384	3.440	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.800%	
20) 2-Butanone-d5	3.931	46	84646	54.879	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	109.760%	
24) Chloroform-d	4.365	84	125725	5.427	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	108.600%	
26) 1,2-Dichloroethane-d4	5.047	65	51632	5.267	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.400%	
32) Benzene-d6	5.063	84	240240	5.054	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.000%	
36) 1,2-Dichloropropane-d6	6.079	67	74386	5.362	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	107.200%	
41) Toluene-d8	7.320	98	197404	4.554	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.000%	
43) trans-1,3-Dichloroprop...	7.632	79	16728	3.719	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	74.400%	
46) 2-Hexanone-d5	8.095	63	64645	47.572	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.140%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46606	5.453	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	109.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	63461	5.703	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	114.000%	
Target Compounds						Qvalue
16) Methylene chloride	2.526	84	12032	0.820	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026485.D
Acq On : 21 Jun 2022 13:56
Operator : SY/MD
Sample : N3358-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 22 04:42:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

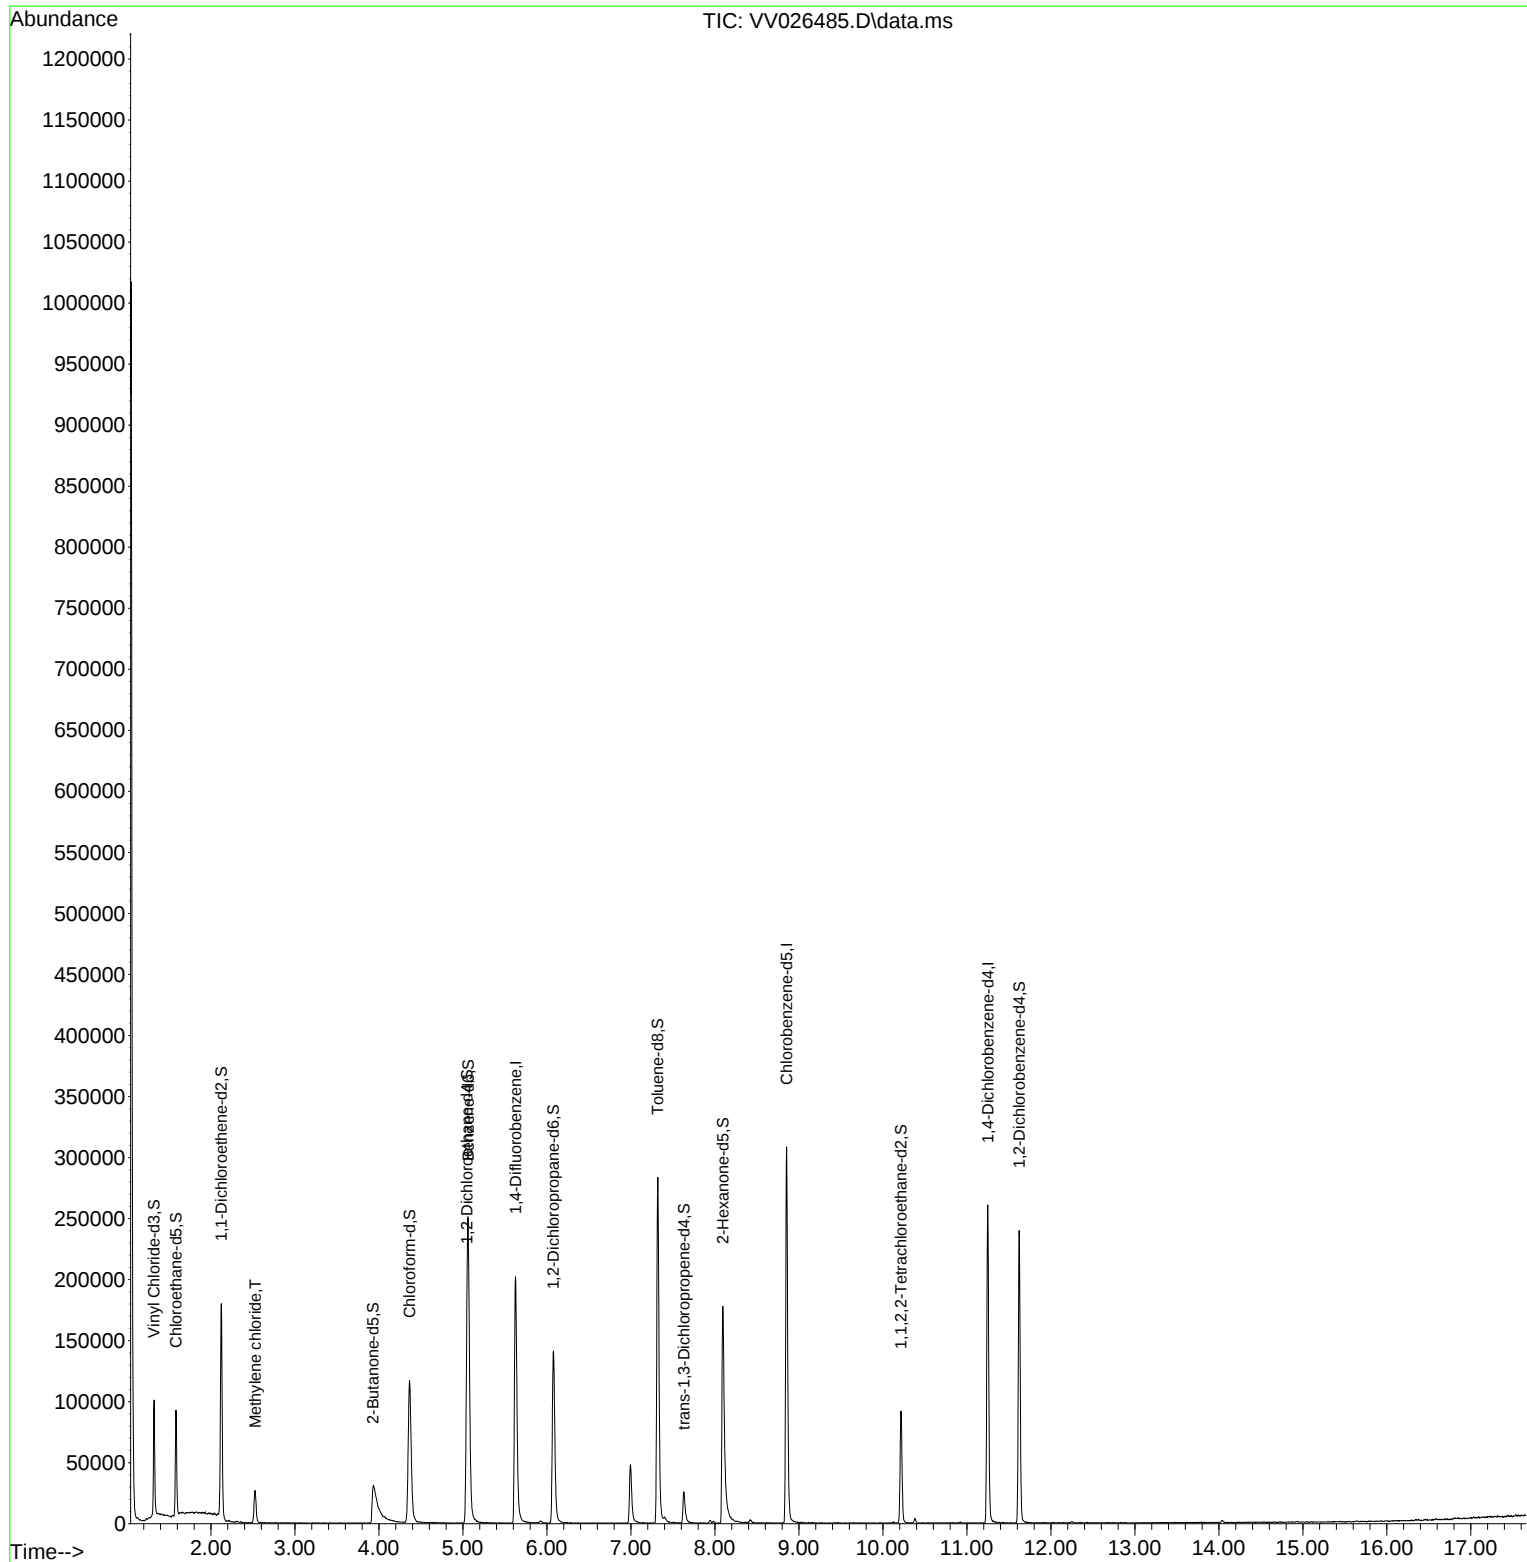

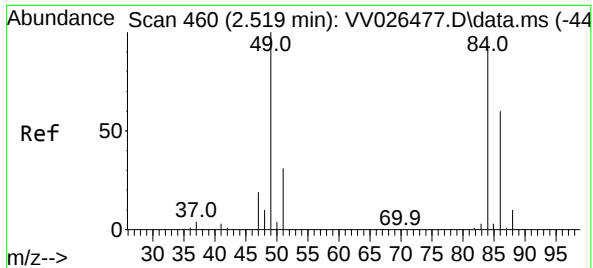

#16
Methylene chloride
Concen: 0.820 ug/L
RT: 2.526 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV026485.D
Acq: 21 Jun 2022 13:56

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

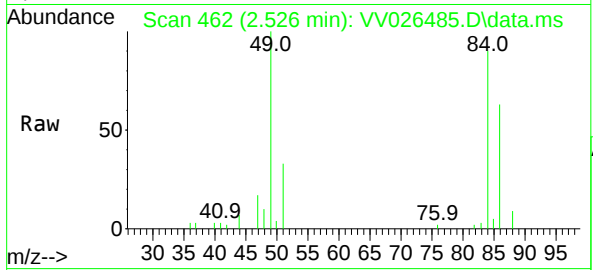

Tgt Ion:	84	Resp:	12032
Ion	Ratio	Lower	Upper
84	100		
86	70.5	44.0	81.8
49	111.6	77.3	143.7

