

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062122\
 Data File : VW026489.D
 Acq On : 21 Jun 2022 15:28
 Operator : SY/MD
 Sample : N3355-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C6

Quant Time: Jun 22 04:43:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.632	114	166947	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	160045	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66105	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.326	65	56180	3.874	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.400%
7) Chloroethane-d5	1.587	69	50774	4.453	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.000%
11) 1,1-Dichloroethene-d2	2.127	63	85513	3.434	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%
20) 2-Butanone-d5	3.937	46	72643	51.341	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.680%
24) Chloroform-d	4.371	84	117706	5.538	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.800%
26) 1,2-Dichloroethane-d4	5.050	65	48847	5.432	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.600%
32) Benzene-d6	5.066	84	219783	5.137	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.800%
36) 1,2-Dichloropropane-d6	6.082	67	67872	5.435	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.800%
41) Toluene-d8	7.323	98	179531	4.602	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	7.632	79	14836	3.664	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.200%
46) 2-Hexanone-d5	8.095	63	61138	49.981	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44049	5.726	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	60758	5.967	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.400%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.982	164	11871	1.431	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026489.D
Acq On : 21 Jun 2022 15:28
Operator : SY/MD
Sample : N3355-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C6


Quant Time: Jun 22 04:43:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

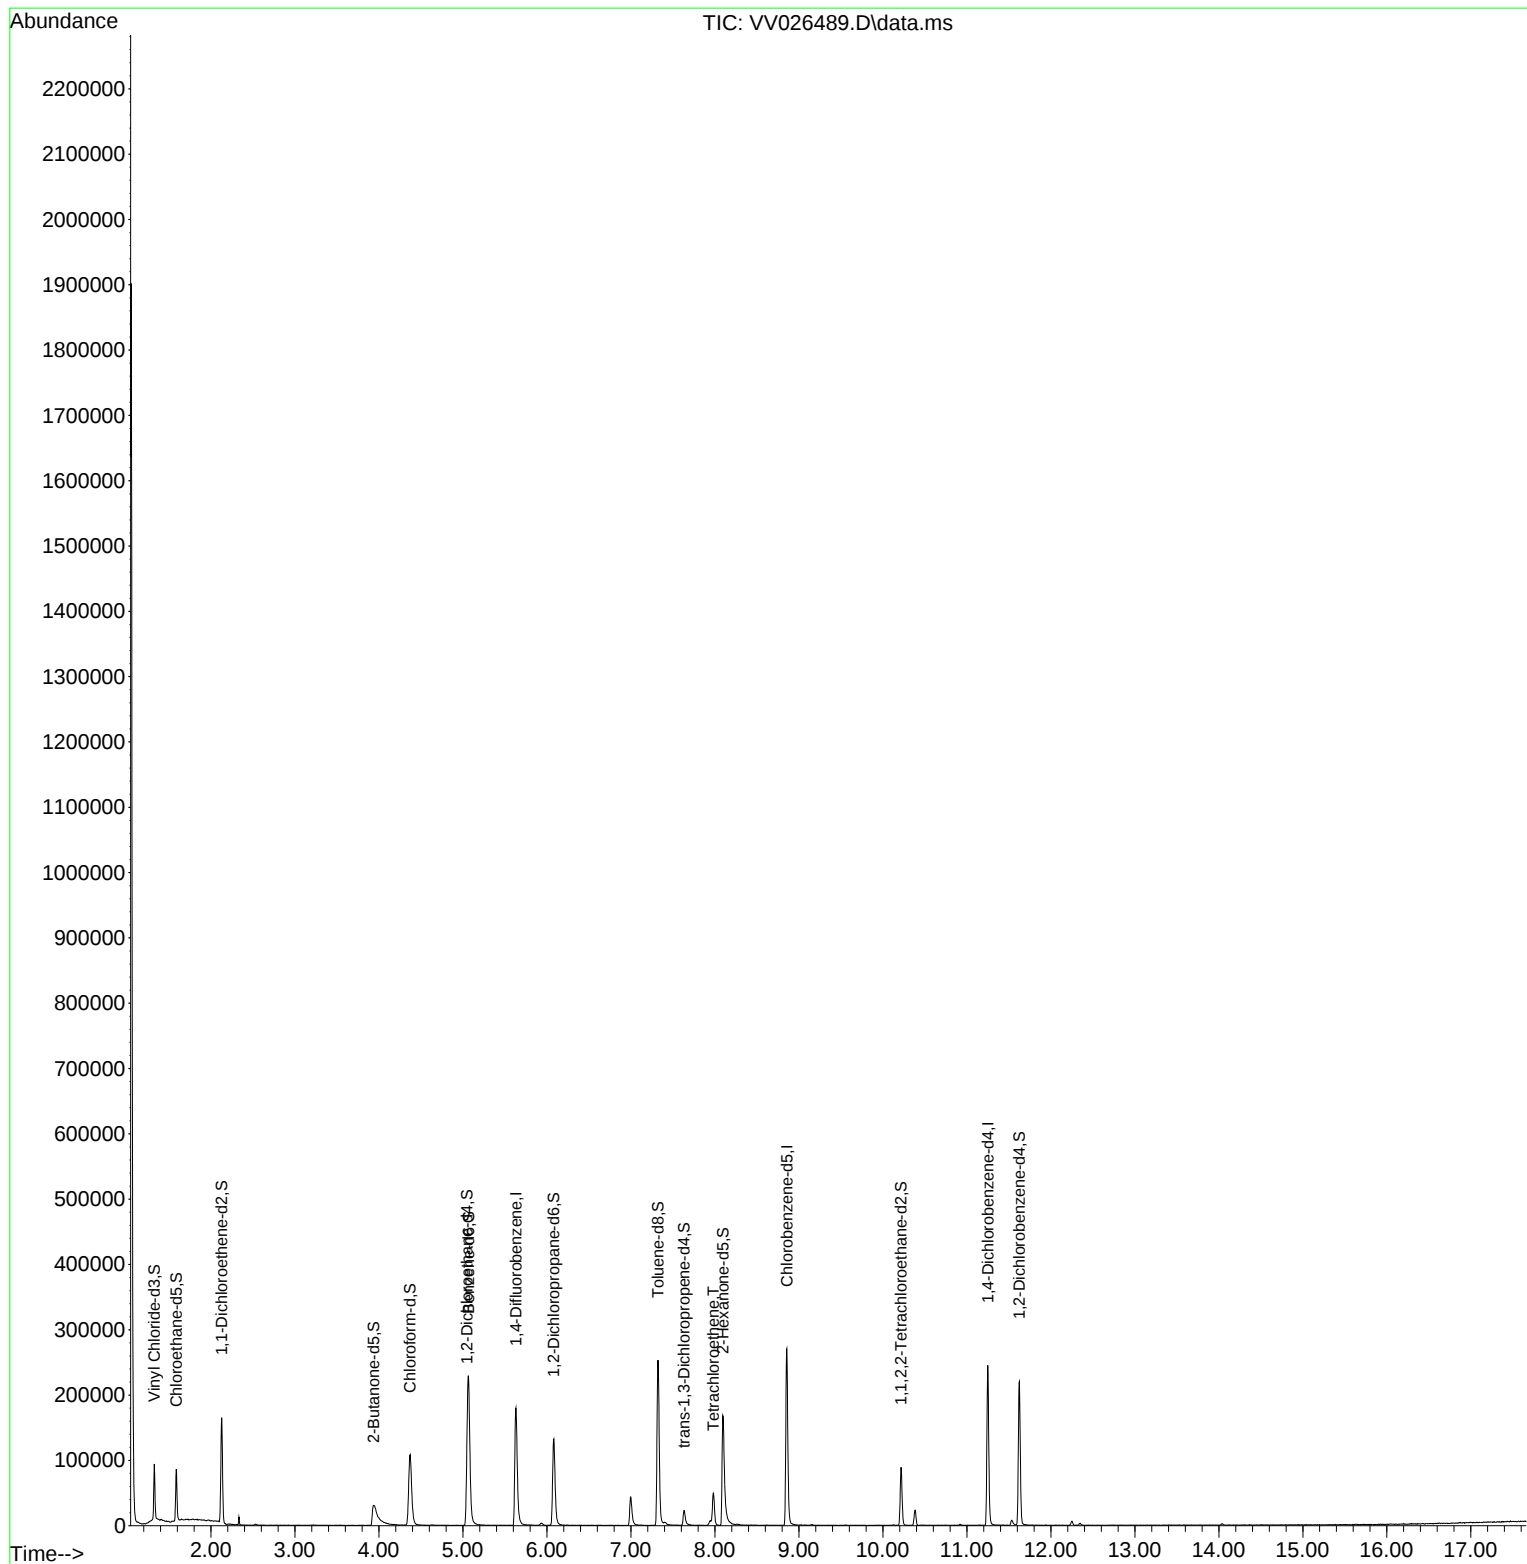

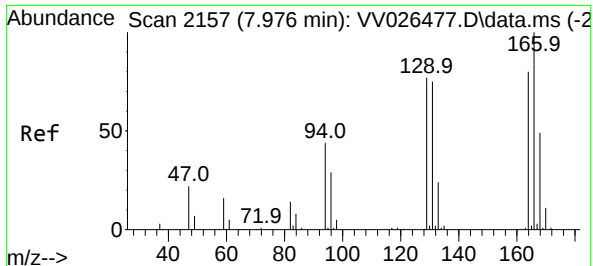

#47
 Tetrachloroethene
 Concen: 1.431 ug/L
 RT: 7.982 min Scan# 2159
 Delta R.T. 0.006 min
 Lab File: VV026489.D
 Acq: 21 Jun 2022 15:28

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C6

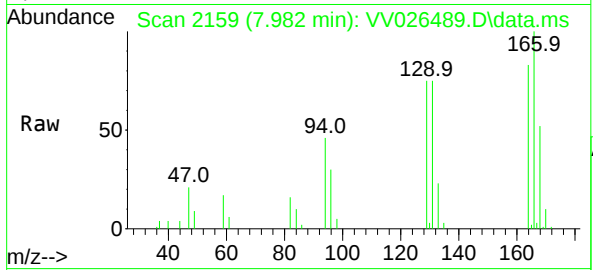

Tgt Ion:	164	Resp:	11871
Ion	Ratio	Lower	Upper
164	100		
129	90.4	67.5	125.3
131	89.8	63.8	118.4
166	120.3	89.5	166.3

