

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062122\
 Data File : VW026493.D
 Acq On : 21 Jun 2022 17:02
 Operator : SY/MD
 Sample : N3355-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D1

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

Quant Time: Jun 22 04:44:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	156764	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	152536	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60734	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	54005	3.966	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.400%	
7) Chloroethane-d5	1.584	69	49738	4.646	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.000%	
11) 1,1-Dichloroethene-d2	2.121	63	80279	3.433	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.600%	
20) 2-Butanone-d5	3.928	46	74788	56.291	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	112.580%	
24) Chloroform-d	4.362	84	112570	5.641	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	112.800%	
26) 1,2-Dichloroethane-d4	5.047	65	46241	5.477	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.600%	
32) Benzene-d6	5.063	84	208775	5.119	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.400%	
36) 1,2-Dichloropropane-d6	6.079	67	65211	5.479	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	109.600%	
41) Toluene-d8	7.320	98	172442	4.637	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	7.632	79	13688	3.547	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	71.000%	
46) 2-Hexanone-d5	8.095	63	57924	49.684	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.360%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41801	5.701	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	114.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	56697	6.061	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	121.200%#	
Target Compounds					Qvalue	
13) Acetone	2.220	43	11785m	11.446	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026493.D
Acq On : 21 Jun 2022 17:02
Operator : SY/MD
Sample : N3355-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
EY0D1

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 06/22/2022
Supervised By :Mahesh Dadoda 06/22/2022


Quant Time: Jun 22 04:44:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

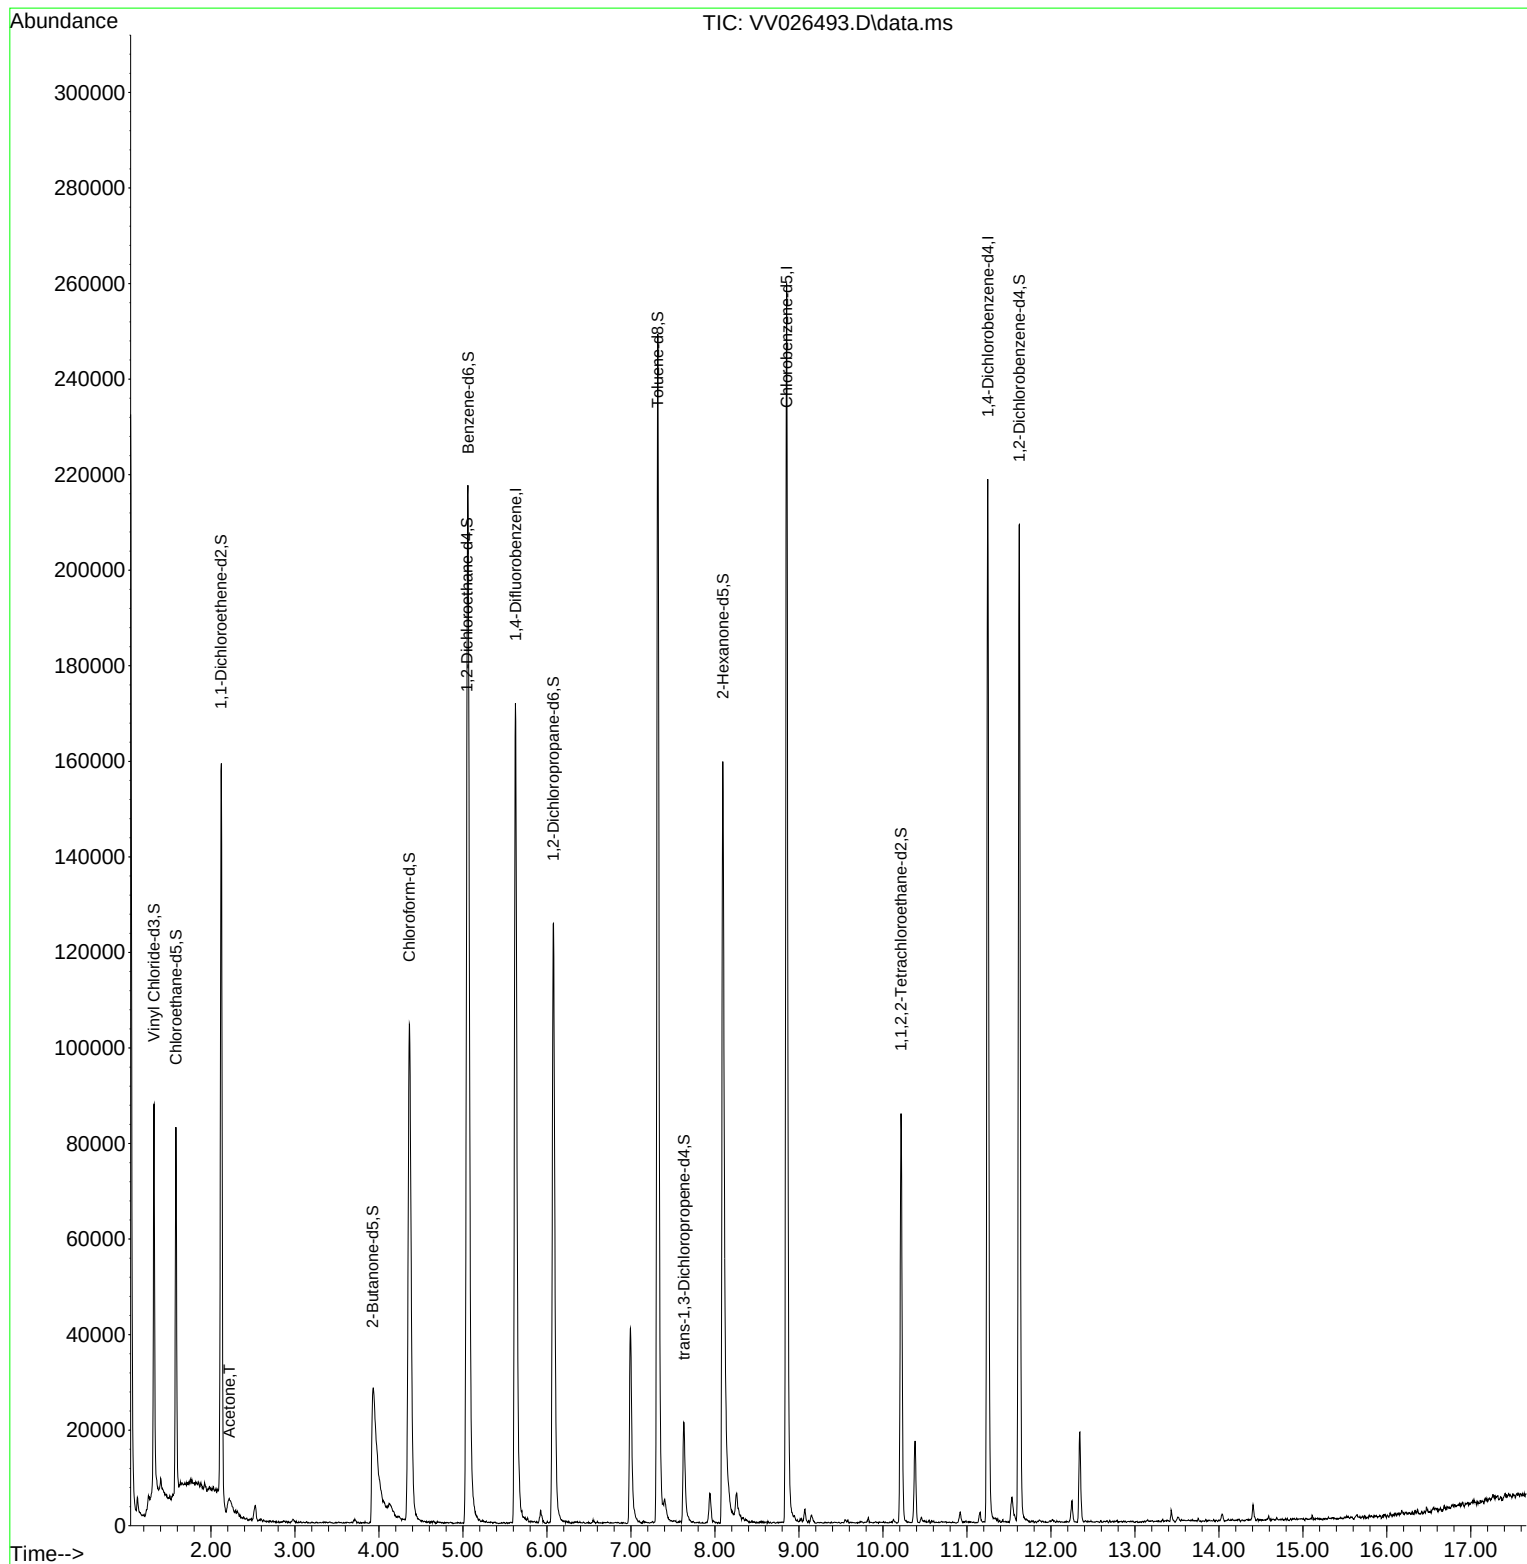

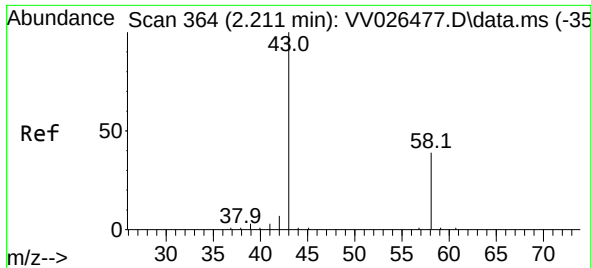

#13
 Acetone
 Concen: 11.446 ug/L m
 RT: 2.220 min Scan# 30
 Delta R.T. 0.010 min
 Lab File: VV026493.D
 Acq: 21 Jun 2022 17:02

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D1

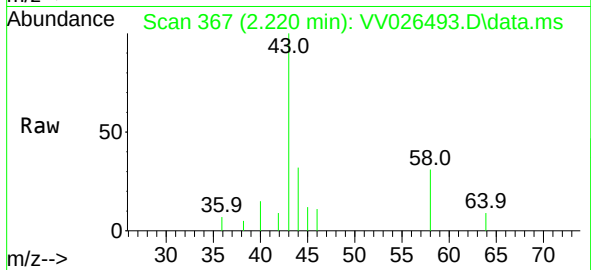

Tgt Ion: 43 Resp: 11785
 Ion Ratio Lower Upper
 43 100
 58 11.1 0.0 60.0

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 06/22/2022
 Supervised By :Mahesh Dadoda 06/22/2022

