

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062122\
 Data File : VW026498.D
 Acq On : 21 Jun 2022 19:02
 Operator : SY/MD
 Sample : N3355-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 22 04:45:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.628	114	157605	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	156041	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62839	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.326	65	55231	4.035	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.600%
7) Chloroethane-d5	1.587	69	52224	4.852	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	2.127	63	84728	3.604	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.000%
20) 2-Butanone-d5	3.931	46	80811	60.499	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.000%
24) Chloroform-d	4.365	84	117879	5.875	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.600%
26) 1,2-Dichloroethane-d4	5.047	65	47217	5.562	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.200%
32) Benzene-d6	5.063	84	220101	5.276	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.600%
36) 1,2-Dichloropropane-d6	6.079	67	69125	5.677	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.600%
41) Toluene-d8	7.320	98	176218	4.632	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
43) trans-1,3-Dichloroprop...	7.632	79	15781	3.997	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	8.095	63	59929	50.250	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.500%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44778	5.970	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	119.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	58880	6.083	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	121.600%#
Target Compounds						Qvalue
16) Methylene chloride	2.529	84	4869	0.383	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026498.D
Acq On : 21 Jun 2022 19:02
Operator : SY/MD
Sample : N3355-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 22 04:45:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 04:36:16 2022
Response via : Initial Calibration

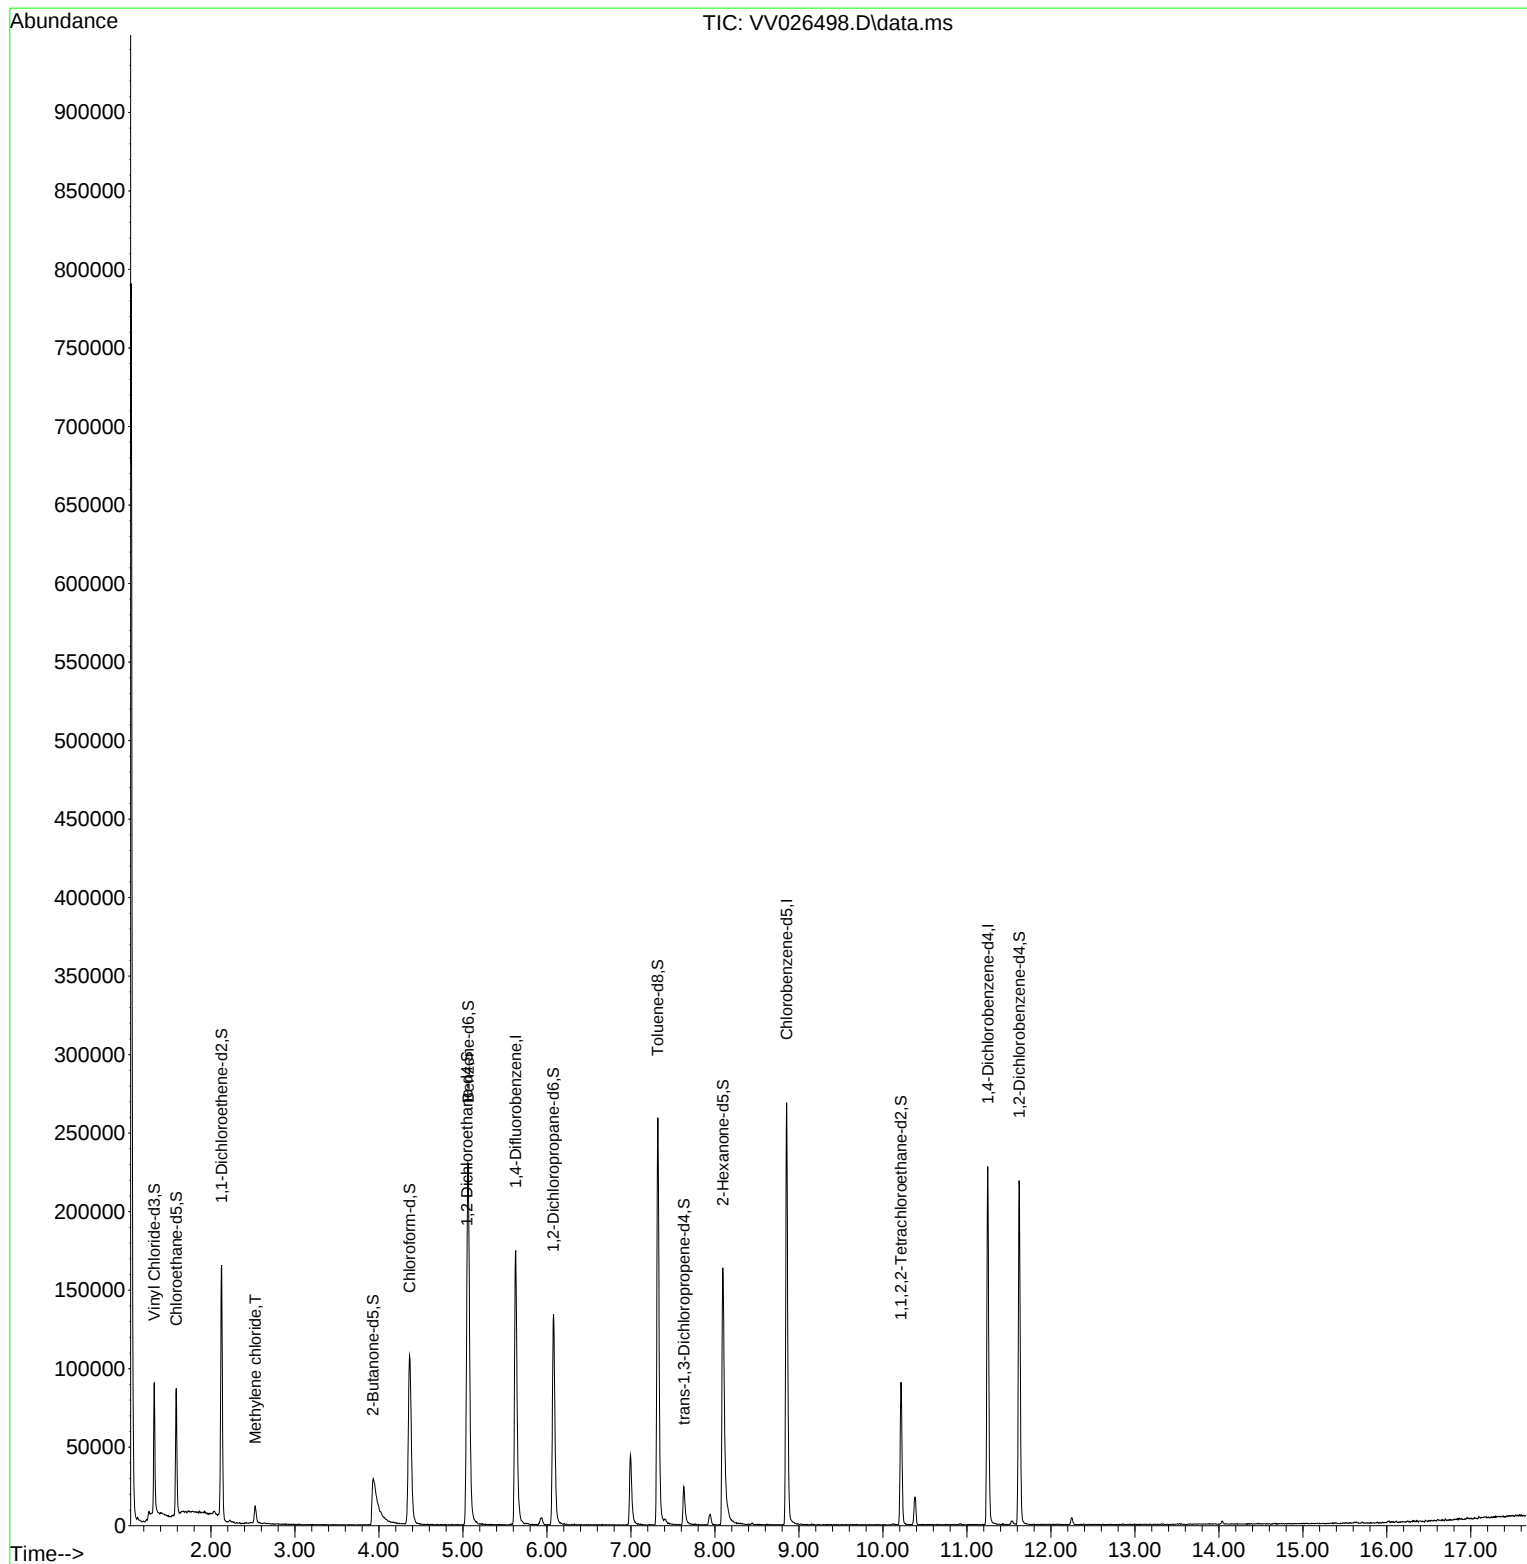

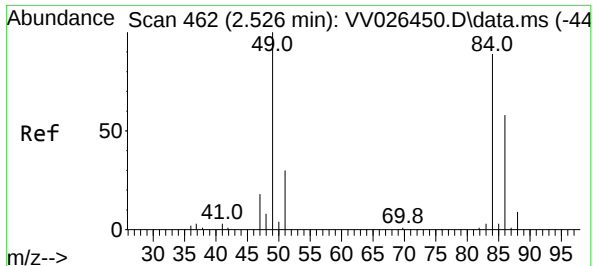

#16
Methylene chloride
Concen: 0.383 ug/L
RT: 2.529 min Scan# 4
Delta R.T. 0.009 min
Lab File: VV026498.D
Acq: 21 Jun 2022 19:02

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

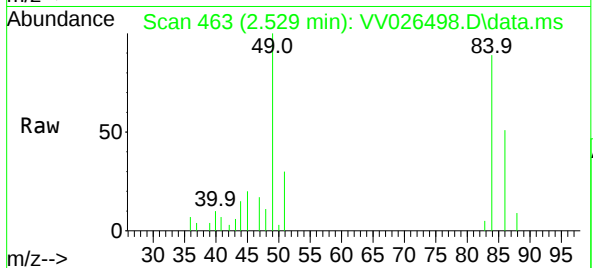

Tgt Ion: 84 Resp: 4869

Ion	Ratio	Lower	Upper
84	100		
86	56.6	44.0	81.8
49	111.9	77.3	143.7

