

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026479.D
 Acq On : 21 Jun 2022 11:33
 Operator : SY/MD
 Sample : N3358-16DL 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	81	88	104	rVB	101220	106229	12.53%	1.919%
2	1.584	162	169	178	rBV	91212	103218	12.17%	1.864%
3	2.124	328	337	352	rVB	185591	266169	31.40%	4.807%
4	2.220	352	367	417	rVB2	18604	92198	10.88%	1.665%
5	2.523	451	461	472	rVB2	10929	18785	2.22%	0.339%
6	3.931	882	899	908	rBV3	40513	117945	13.91%	2.130%
7	4.362	1014	1033	1083	rBV3	256684	847797	100.00%	15.313%
8	5.056	1231	1249	1278	rBV2	269555	668163	78.81%	12.068%
9	5.622	1409	1425	1448	rBV	213964	437283	51.58%	7.898%
10	6.075	1551	1566	1589	rBV2	149177	306077	36.10%	5.528%
11	6.989	1837	1850	1871	rBV	50964	98107	11.57%	1.772%
12	7.317	1941	1952	1972	rBV	305166	535384	63.15%	9.670%
13	7.625	2039	2048	2070	rBV3	26910	50730	5.98%	0.916%
14	8.091	2183	2193	2235	rBV	184261	385847	45.51%	6.969%
15	8.419	2283	2295	2306	rBV3	10920	19160	2.26%	0.346%
16	8.850	2419	2429	2459	rBV	300616	505502	59.63%	9.130%
17	10.030	2785	2796	2813	rBV7	5187	13290	1.57%	0.240%
18	10.214	2843	2853	2874	rBV	93465	149093	17.59%	2.693%
19	11.249	3164	3175	3194	rBV	271056	424041	50.02%	7.659%
20	11.622	3280	3291	3307	rBV	250636	391598	46.19%	7.073%




Sum of corrected areas: 5536616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026479.D
Acq On : 21 Jun 2022 11:33
Operator : SY/MD
Sample : N3358-16DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

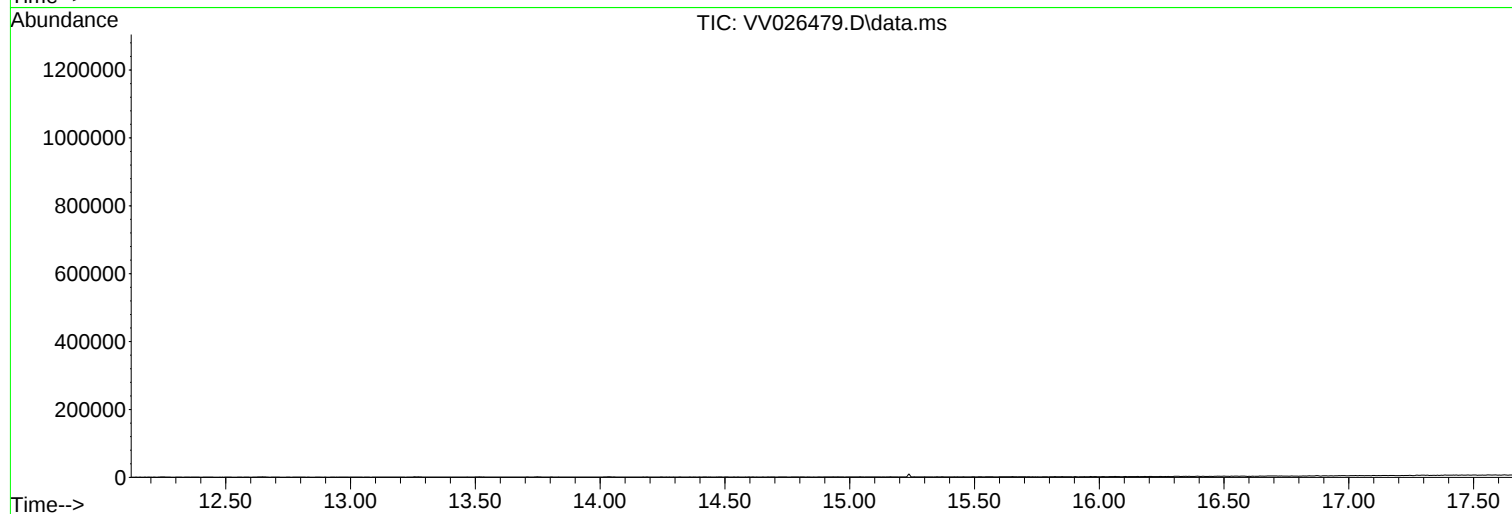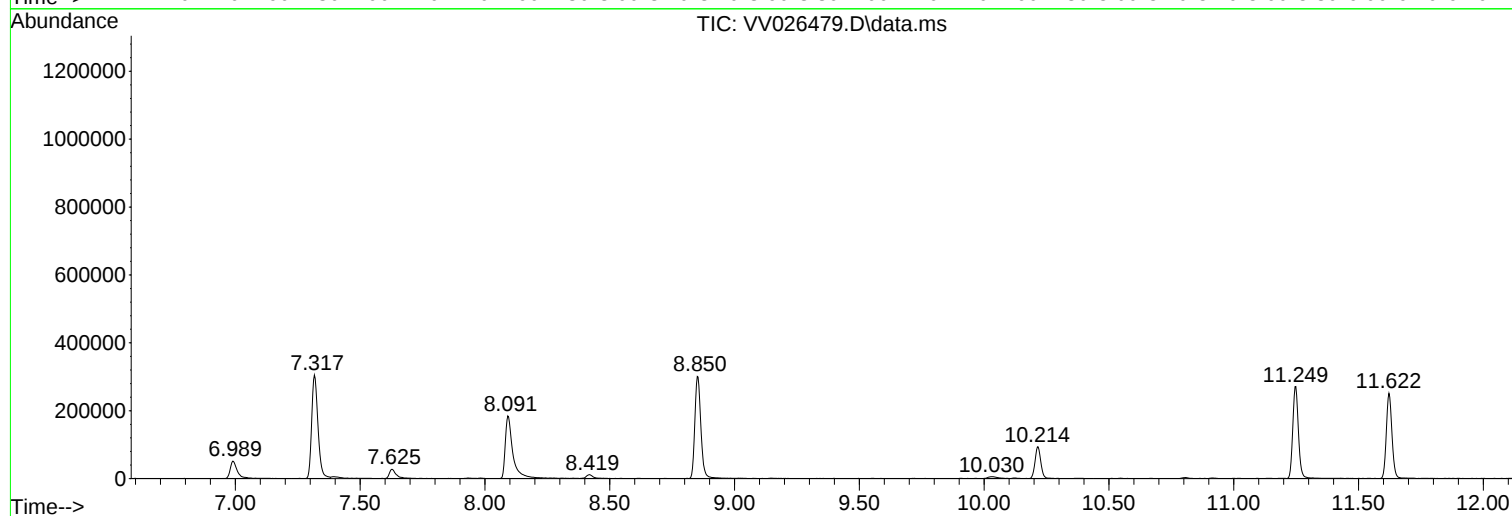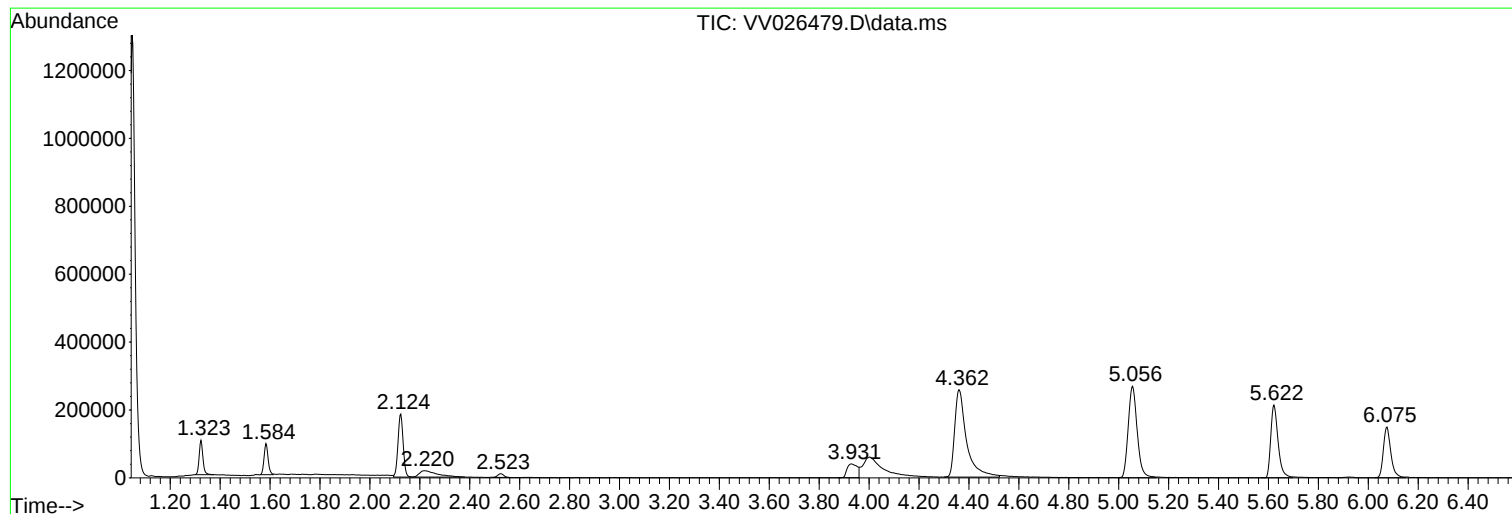

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026479.D
Acq On : 21 Jun 2022 11:33
Operator : SY/MD
Sample : N3358-16DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026479.D
Acq On : 21 Jun 2022 11:33
Operator : SY/MD
Sample : N3358-16DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc