

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026480.D
 Acq On : 21 Jun 2022 11:57
 Operator : SY/MD
 Sample : N3358-15DL 500X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	81	88	104	rBV	97821	102625	12.47%	1.901%
2	1.587	162	170	179	rBV	86748	99664	12.11%	1.846%
3	2.124	327	337	353	rVB	182309	265851	32.30%	4.923%
4	2.224	353	368	404	rBV2	17231	82007	9.96%	1.519%
5	2.526	452	462	473	rVB2	8920	15515	1.89%	0.287%
6	3.941	884	902	911	rBV3	40066	121026	14.71%	2.241%
7	4.365	1016	1034	1090	rBV5	242131	822999	100.00%	15.241%
8	5.059	1235	1250	1285	rBV2	261039	647571	78.68%	11.993%
9	5.625	1415	1426	1455	rBV	213322	441970	53.70%	8.185%
10	6.079	1554	1567	1591	rBV	143580	298706	36.29%	5.532%
11	6.995	1841	1852	1878	rBV	50273	97061	11.79%	1.797%
12	7.320	1941	1953	1975	rBV	293837	515936	62.69%	9.555%
13	7.628	2040	2049	2073	rBV2	26919	50348	6.12%	0.932%
14	8.095	2181	2194	2226	rBV	174222	365400	44.40%	6.767%
15	8.423	2284	2296	2312	rBV3	14034	25620	3.11%	0.474%
16	8.854	2419	2430	2453	rBV	312075	504423	61.29%	9.342%
17	10.217	2843	2854	2868	rBV	90901	144460	17.55%	2.675%
18	11.249	3163	3175	3196	rBV	270424	418967	50.91%	7.759%
19	11.622	3278	3291	3313	rBV	242526	379640	46.13%	7.031%




Sum of corrected areas: 5399789

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026480.D
Acq On : 21 Jun 2022 11:57
Operator : SY/MD
Sample : N3358-15DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

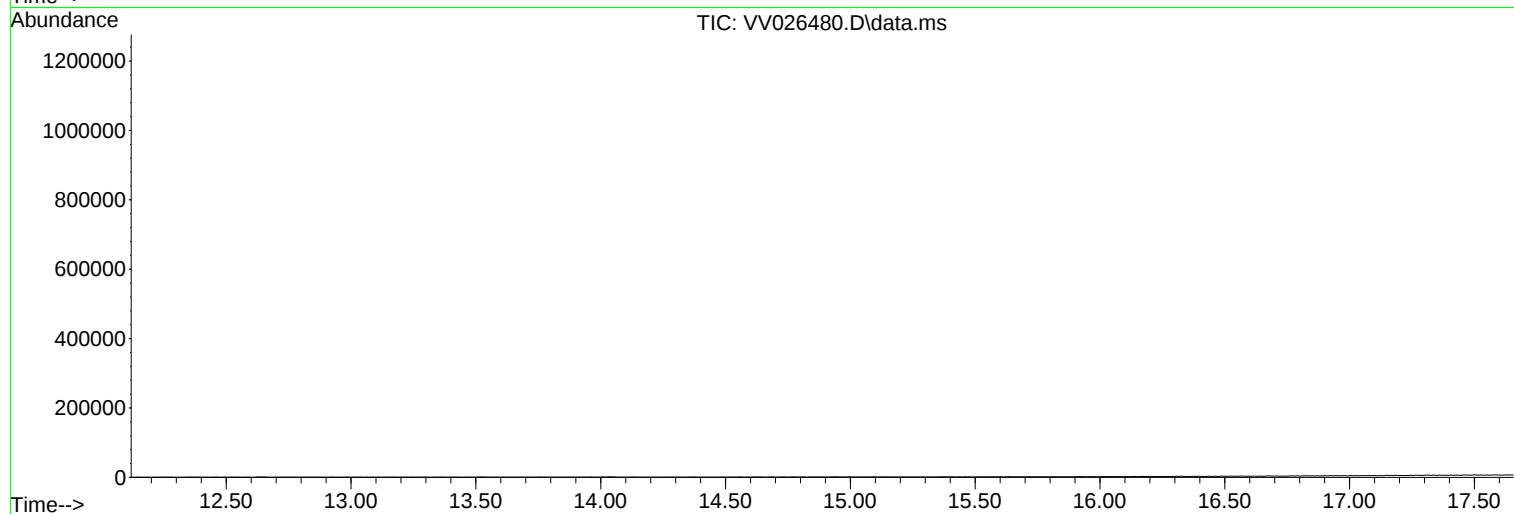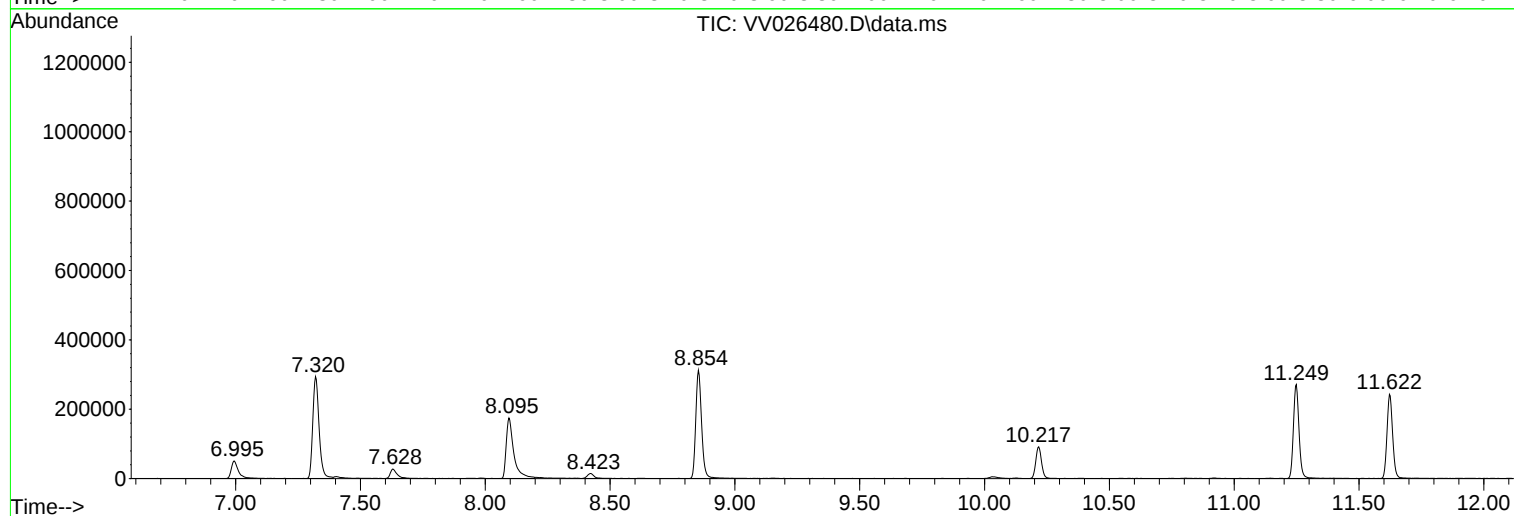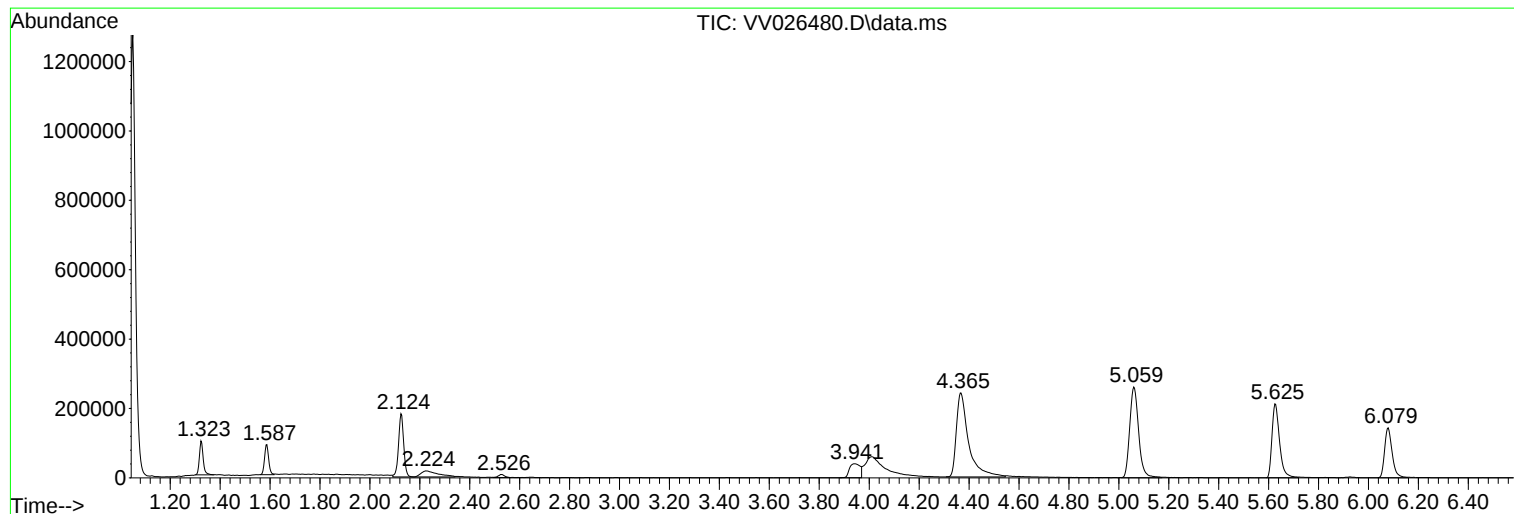

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026480.D
Acq On : 21 Jun 2022 11:57
Operator : SY/MD
Sample : N3358-15DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026480.D
Acq On : 21 Jun 2022 11:57
Operator : SY/MD
Sample : N3358-15DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc